
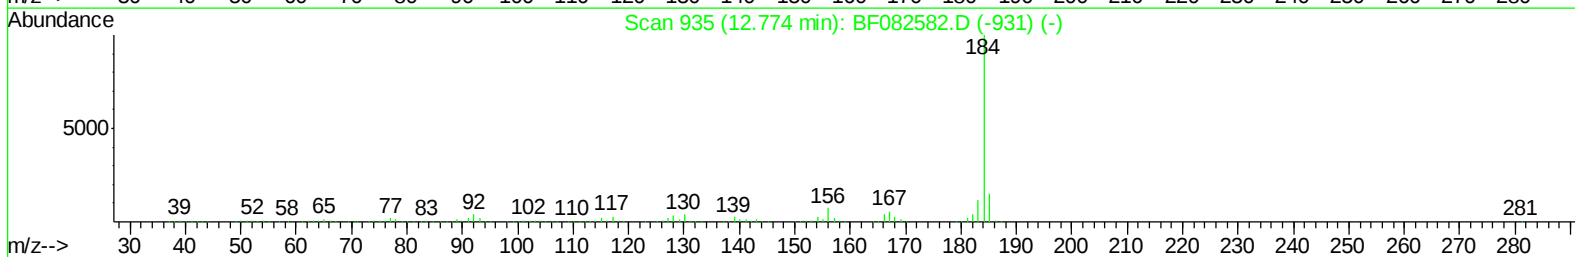
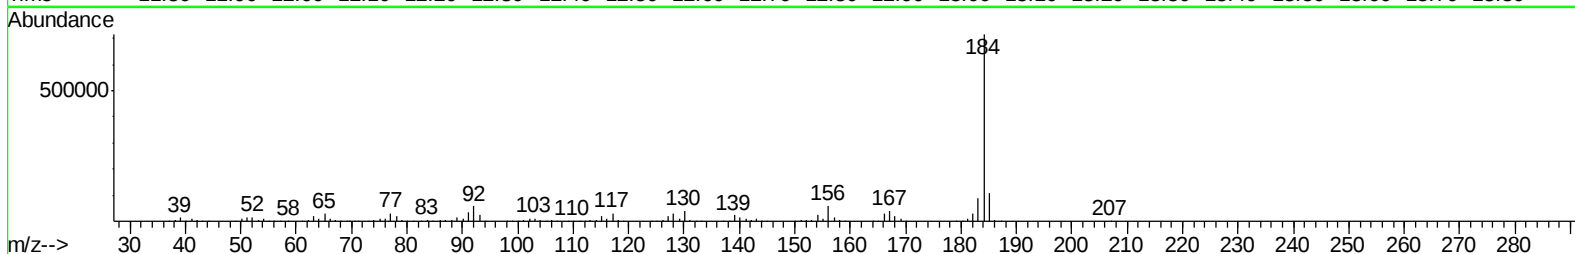


Data Path : Z:\HPCHEM1\BNA_F\Data\BF103015\
Data File : BF082625.D
Acq On : 31 Oct 2015 17:01
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:21:06 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

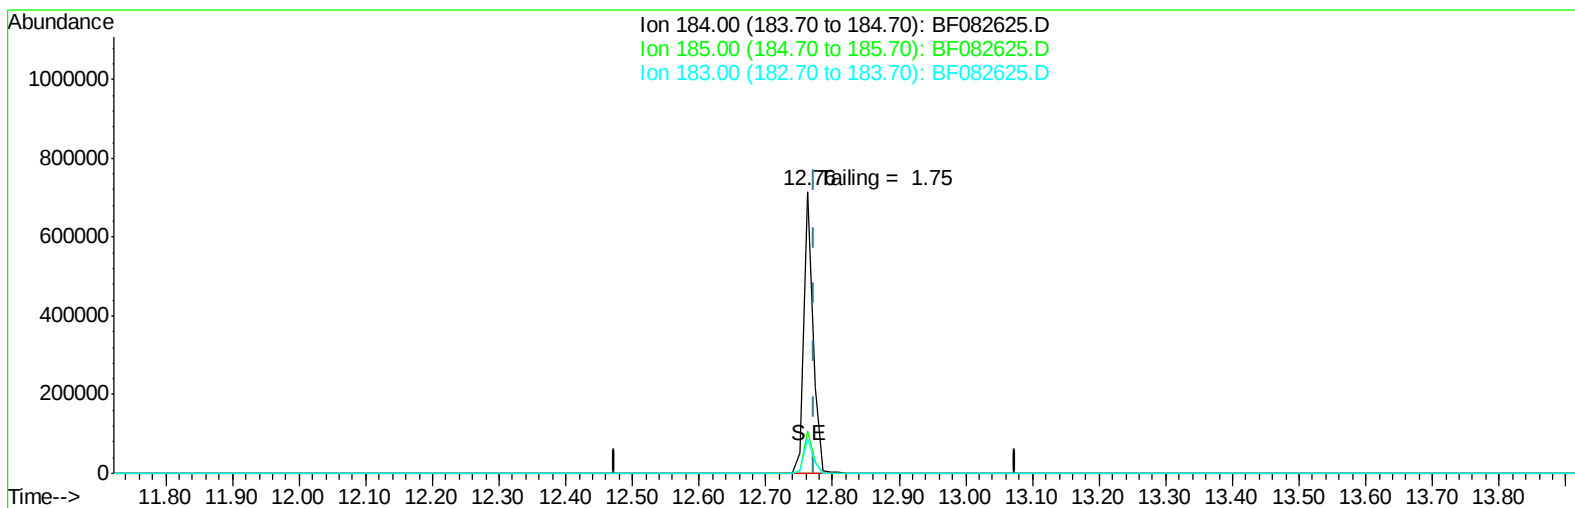

TIC: BF082625.D

(76) Benzidine

12.762min (-0.012) 0.00ng

response 688535

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	15.19
183.00	12.00	12.30
0.00	0.00	0.00