

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103015\
 Data File : BF082588.D
 Acq On : 30 Oct 2015 23:00
 Operator : UM/IZ
 Sample : PB86309BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB86309BL

Quant Time: Oct 31 03:25:10 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 31 00:17:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	184244	20.00	ng	-0.01
21) Naphthalene-d8	8.19	136	755727	20.00	ng	0.00
38) Acenaphthene-d10	9.95	164	401431	20.00	ng	0.00
63) Phenanthrene-d10	11.44	188	736438	20.00	ng	0.00
75) Chrysene-d12	14.07	240	565070	20.00	ng	-0.01
86) Perylene-d12	15.53	264	432917	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	1321389	108.02	ng	0.01
7) Phenol-d6	6.53	99	1923656	118.37	ng	0.00
23) Nitrobenzene-d5	7.46	82	1265706	68.39	ng	-0.01
41) 2,4,6-Tribromophenol	10.74	330	537687	122.39	ng	0.00
44) 2-Fluorobiphenyl	9.28	172	2211984	78.23	ng	0.00
78) Terphenyl-d14	13.03	244	1896291	73.44	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103015\
Data File : BF082588.D
Acq On : 30 Oct 2015 23:00
Operator : UM/IZ
Sample : PB86309BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86309BL

Quant Time: Oct 31 03:25:10 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

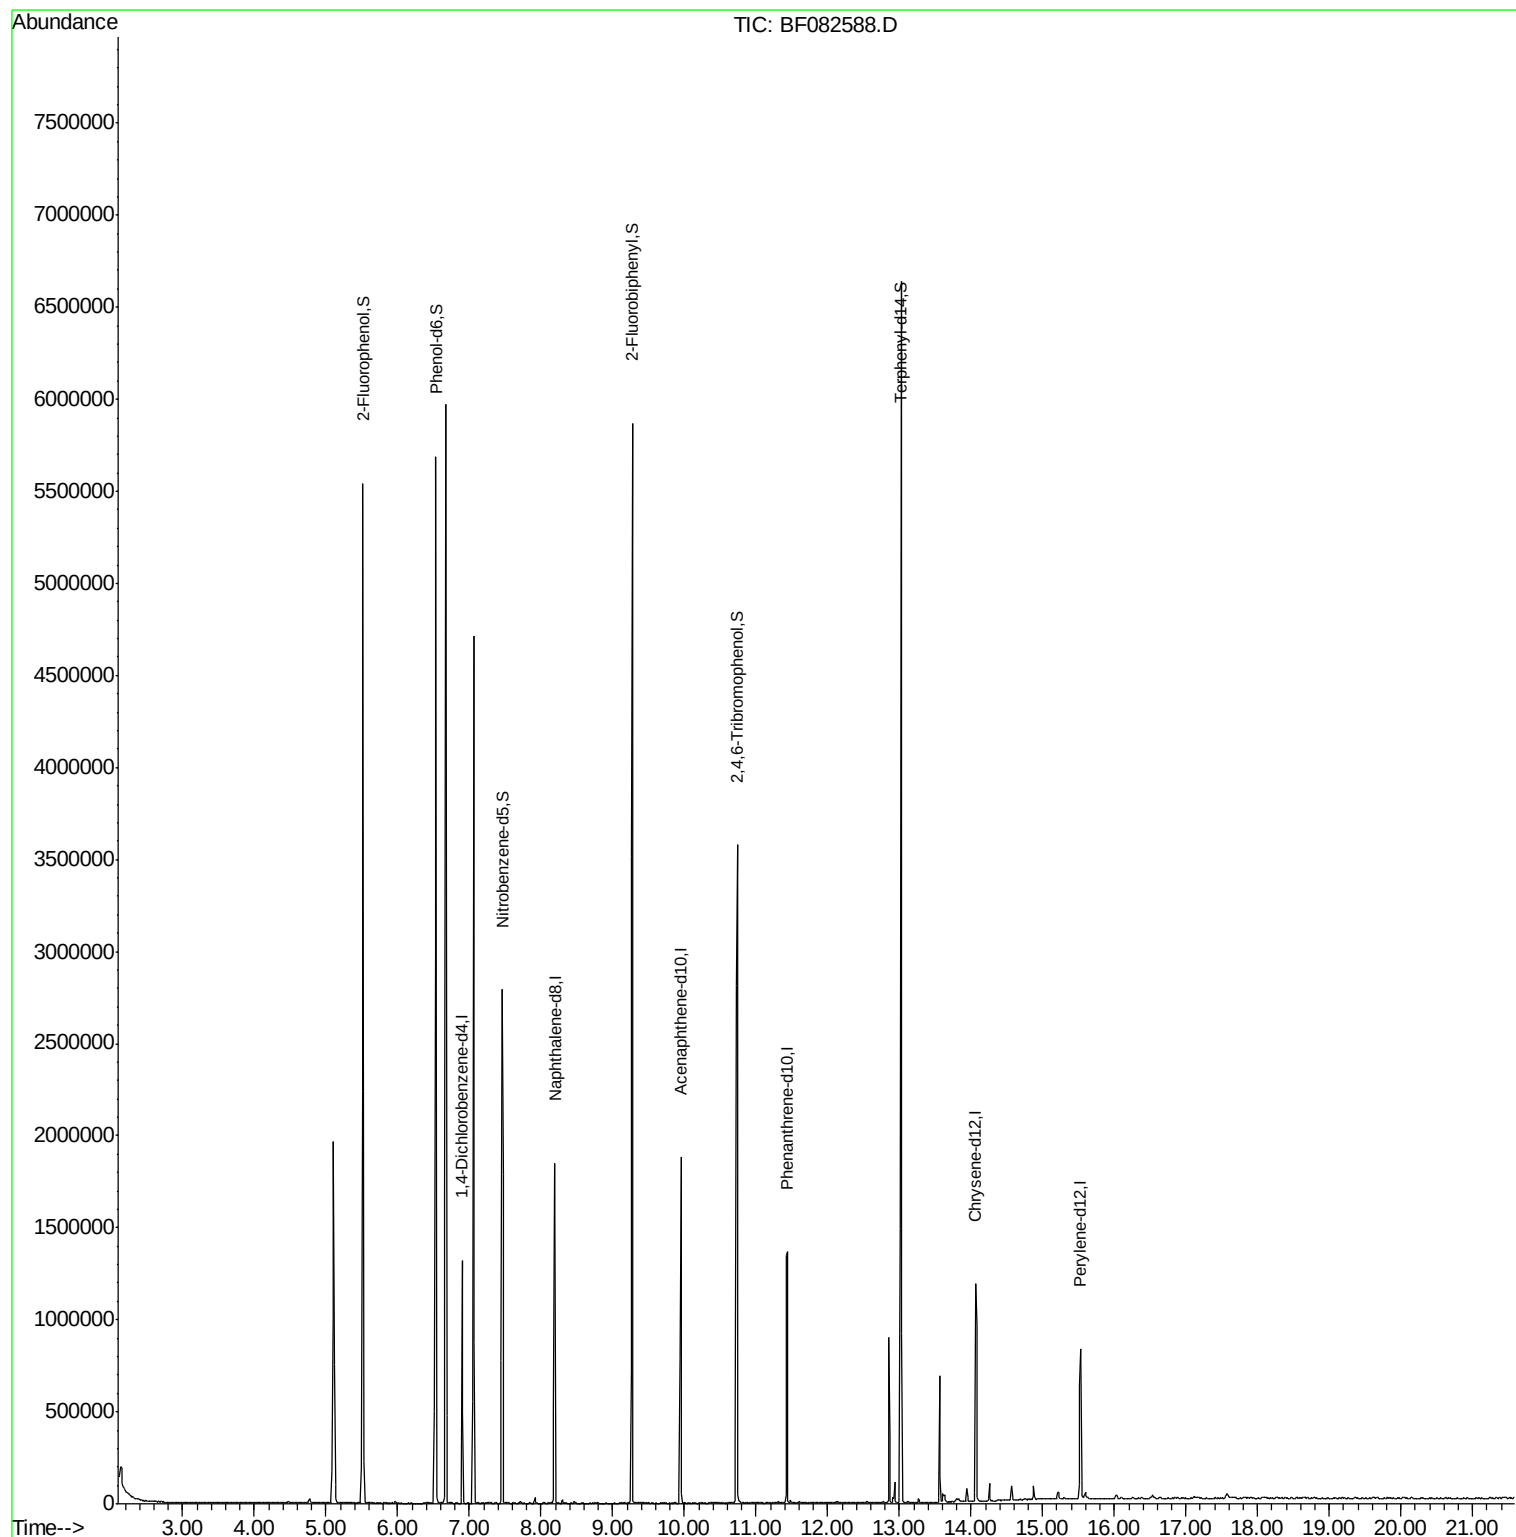

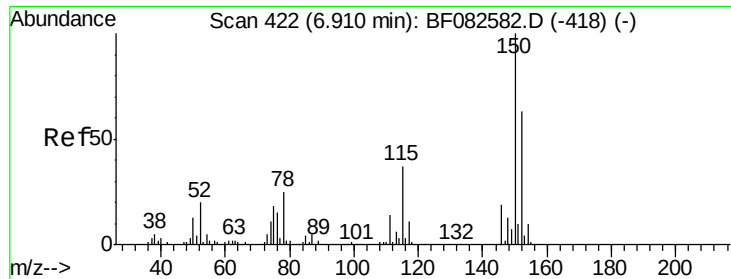


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.90 min Scan# 421
Delta R.T. -0.01 min
Lab File: BF082588.D
Acq: 30 Oct 2015 23:00

Instrument :
BNA_F
ClientSampleId :
PB86309BL

Tgt Ion:152 Resp: 184244
Ion Ratio Lower Upper
152 100
150 162.2 127.0 190.4
115 79.0 47.0 70.6#

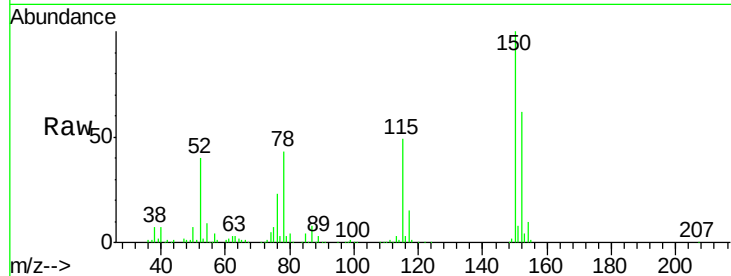


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

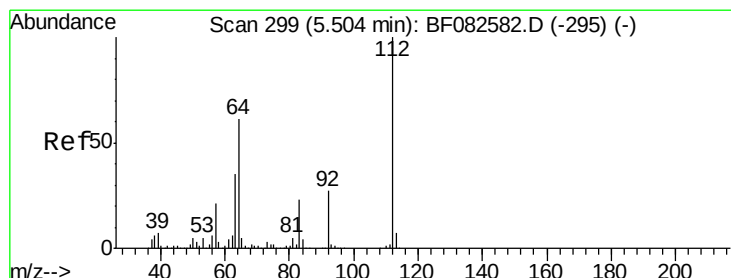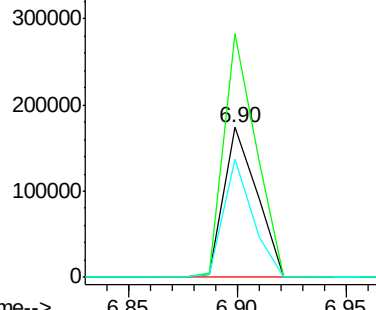



#5


2-Fluorophenol
Concen: 108.02 ng
RT: 5.52 min Scan# 300
Delta R.T. 0.01 min
Lab File: BF082588.D
Acq: 30 Oct 2015 23:00

Tgt Ion:112 Resp: 1321389
Ion Ratio Lower Upper
112 100
64 73.2 48.9 73.3
63 42.1 28.1 42.1

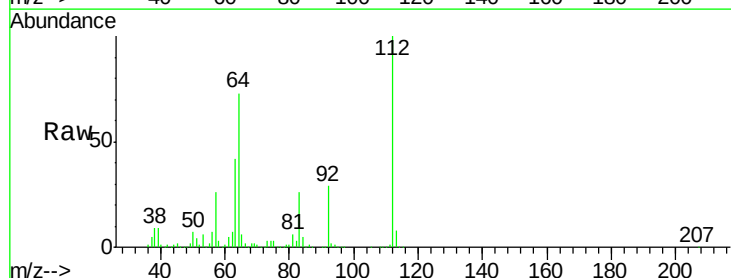

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

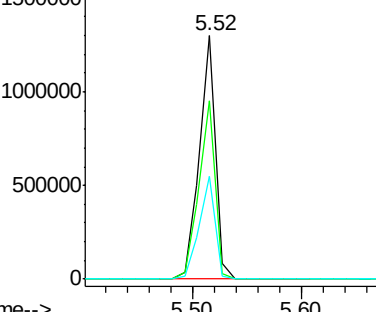



#7

Phenol-d6

Concen: 118.37 ng

RT: 6.53 min Scan# 389

Delta R.T. -0.00 min

Lab File: BF082588.D

Acq: 30 Oct 2015 23:00

Instrument :

BNA_F

ClientSampleId :

PB86309BL


Tgt Ion: 99 Resp: 1923656

Ion Ratio Lower Upper

99 100

42 24.4 19.2 28.8




71 45.6 35.0 52.4

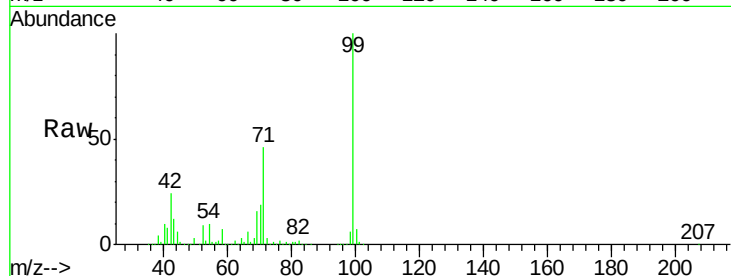

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

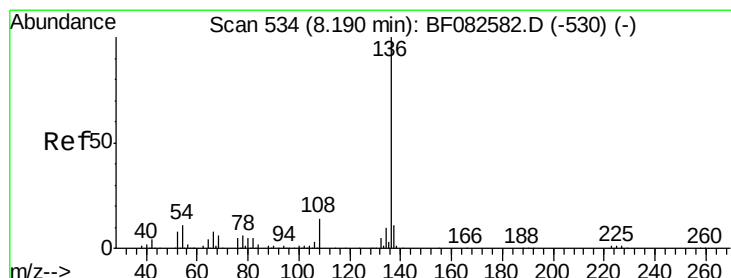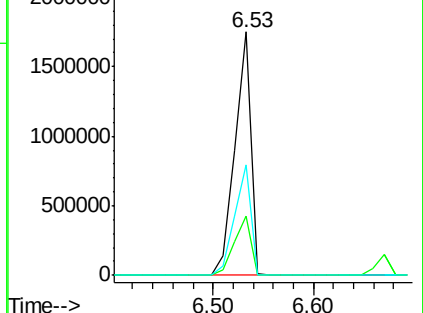

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.19 min Scan# 534

Delta R.T. -0.00 min

Lab File: BF082588.D

Acq: 30 Oct 2015 23:00

Tgt Ion: 136 Resp: 755727


Ion Ratio Lower Upper

136 100

137 11.4 9.1 13.7

54 9.0 9.1 13.7#

68 5.2 4.8 7.2


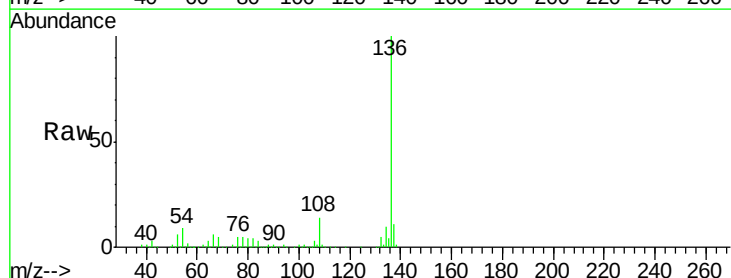



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



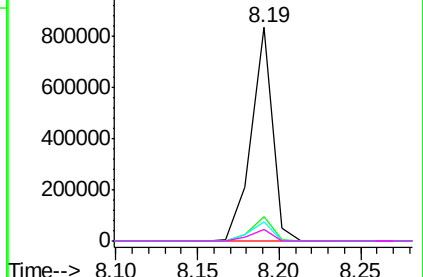





#23
 Nitrobenzene-d5
 Concen: 68.39 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.01 min
 Lab File: BF082588.D
 Acq: 30 Oct 2015 23:00




Instrument :
 BNA_F
 ClientSampleId :
 PB86309BL


Tgt Ion: 82 Resp: 1265706
 Ion Ratio Lower Upper
 82 100
 128 32.5 26.8 40.2
 54 58.0 45.7 68.5

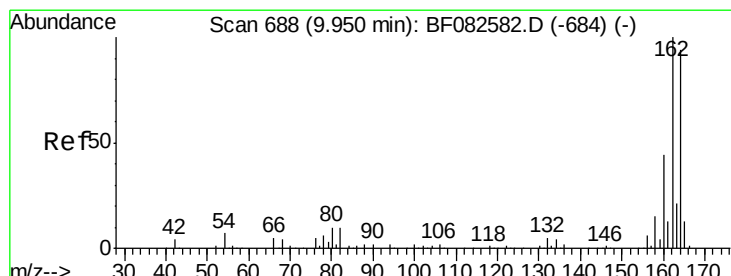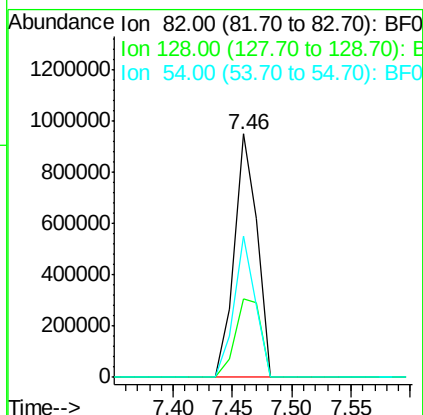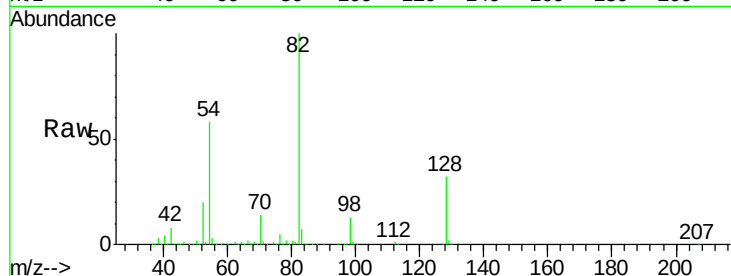

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.95 min Scan# 688
 Delta R.T. -0.00 min
 Lab File: BF082588.D
 Acq: 30 Oct 2015 23:00

Tgt Ion: 164 Resp: 401431
 Ion Ratio Lower Upper
 164 100
 162 104.4 84.9 127.3
 160 47.1 37.5 56.3

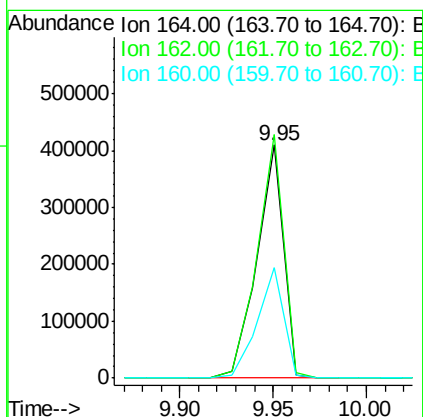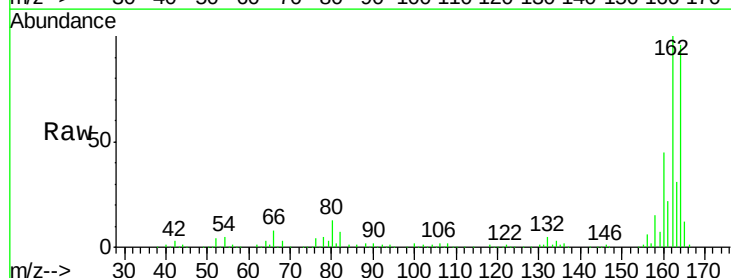


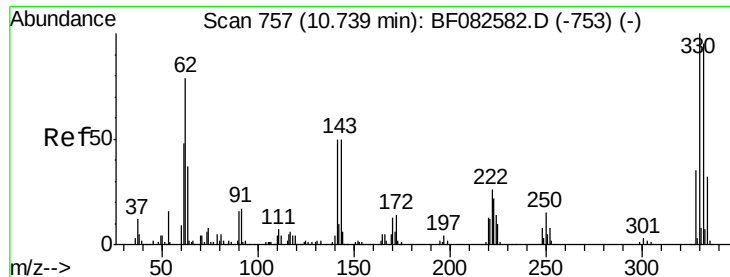




#41
 2,4,6-Tribromophenol
 Concen: 122.39 ng
 RT: 10.74 min Scan# 757
 Delta R.T. -0.00 min
 Lab File: BF082588.D
 Acq: 30 Oct 2015 23:00

Instrument :
 BNA_F
 ClientSampleId :
 PB86309BL

Tgt Ion:330 Resp: 537687
 Ion Ratio Lower Upper
 330 100
 332 97.0 76.6 114.8
 141 39.5 41.2 61.8#

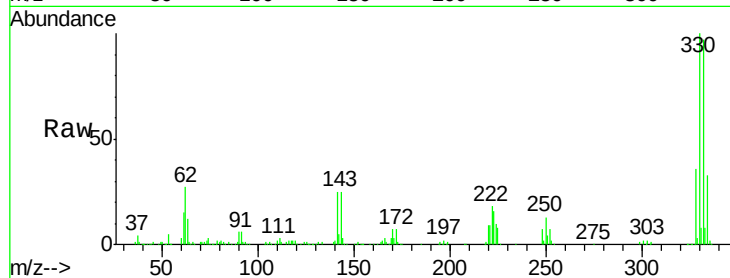


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

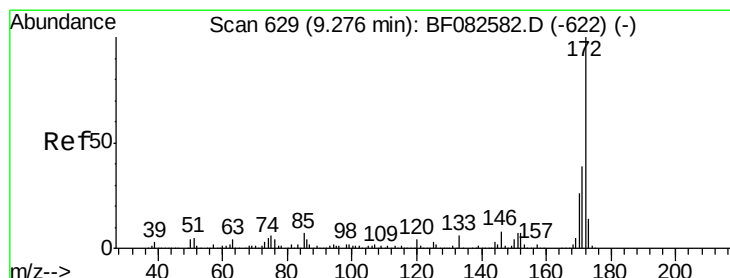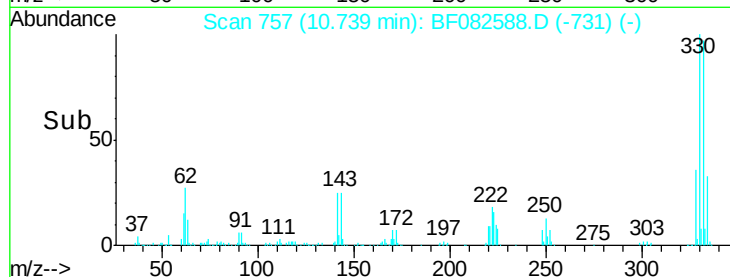
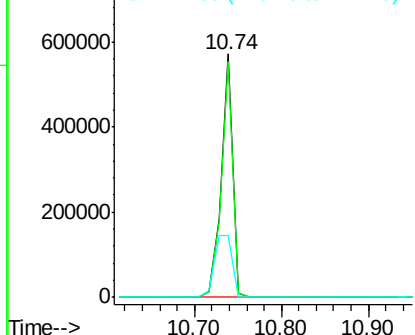



#44
 2-Fluorobiphenyl
 Concen: 78.23 ng
 RT: 9.28 min Scan# 629
 Delta R.T. -0.00 min
 Lab File: BF082588.D
 Acq: 30 Oct 2015 23:00

Tgt Ion:172 Resp: 2211984
 Ion Ratio Lower Upper
 172 100
 171 37.9 30.8 46.2
 170 25.8 21.2 31.8

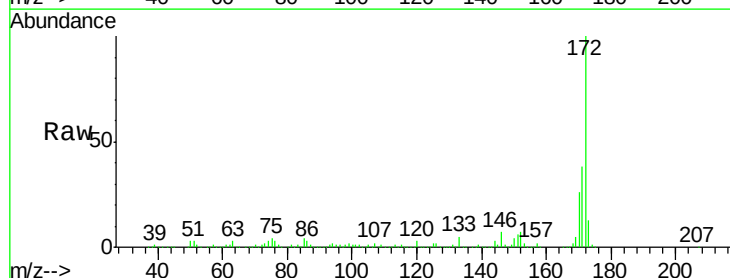

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

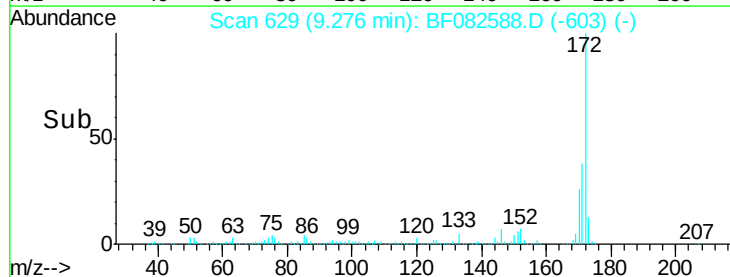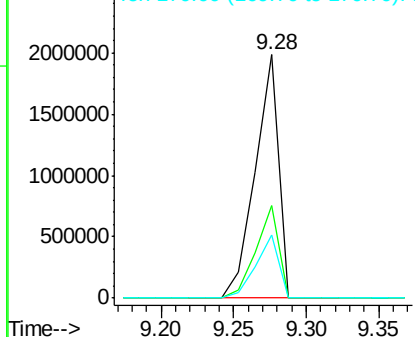

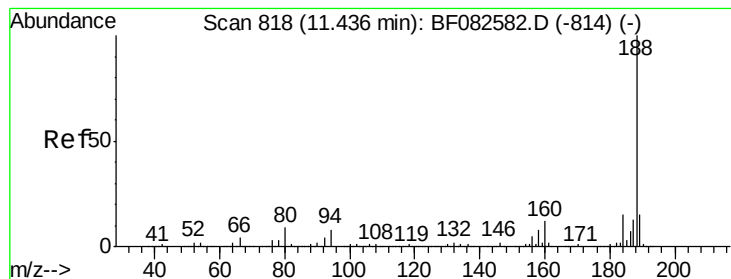

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.44 min Scan# 818

Delta R.T. -0.00 min

Lab File: BF082588.D

Acq: 30 Oct 2015 23:00

Instrument :

BNA_F

ClientSampleId :

PB86309BL


Tgt Ion:188 Resp: 736438

Ion Ratio Lower Upper

188 100

94 5.2 6.1 9.1#




80 5.4 7.0 10.6#

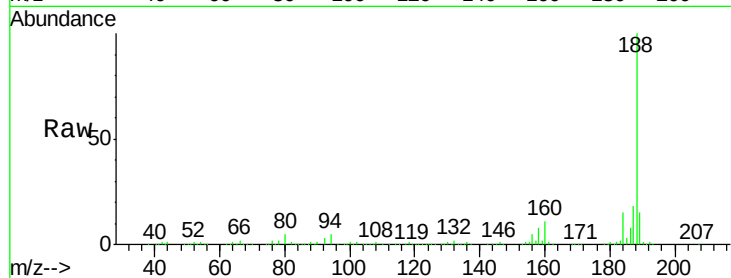

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

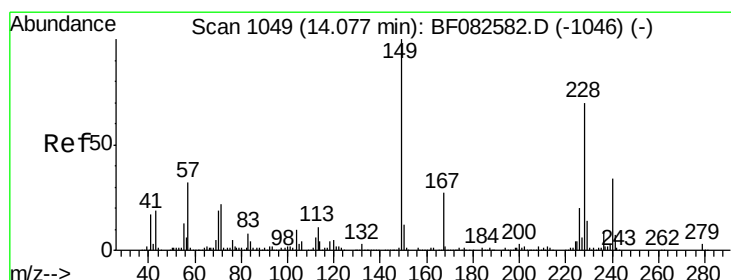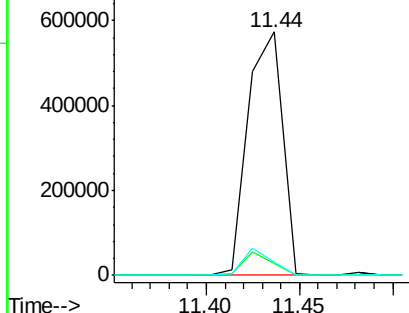

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.07 min Scan# 1048

Delta R.T. -0.01 min

Lab File: BF082588.D

Acq: 30 Oct 2015 23:00


Tgt Ion:240 Resp: 565070

Ion Ratio Lower Upper

240 100

120 12.0 10.9 16.3



236 26.6 21.6 32.4

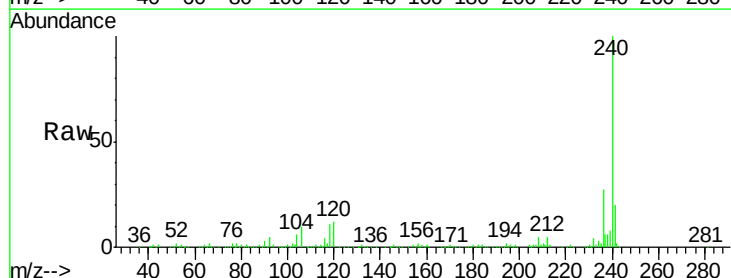


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

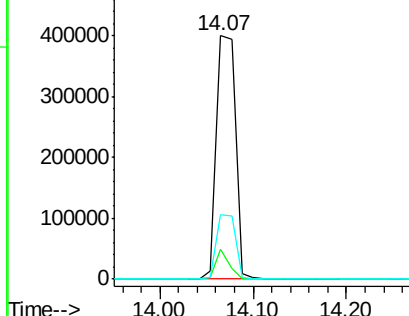

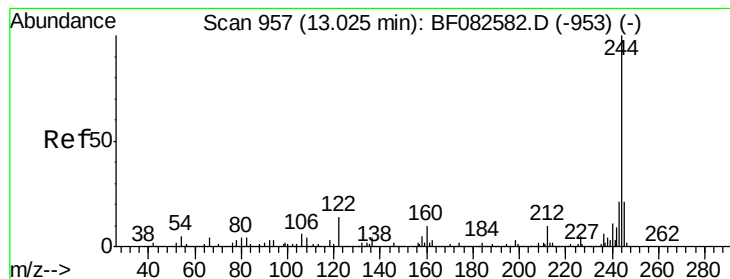

#78

Terphenyl-d14

Concen: 73.44 ng

RT: 13.03 min Scan# 957

Delta R.T. -0.00 min

Lab File: BF082588.D

Acq: 30 Oct 2015 23:00

Instrument :

BNA_F

ClientSampleId :

PB86309BL


Tgt Ion:244 Resp: 1896291

Ion Ratio Lower Upper

244 100

212 8.9 7.6 11.4




122 12.6 11.3 16.9

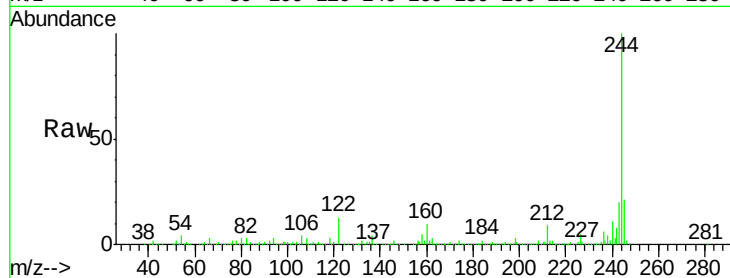

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

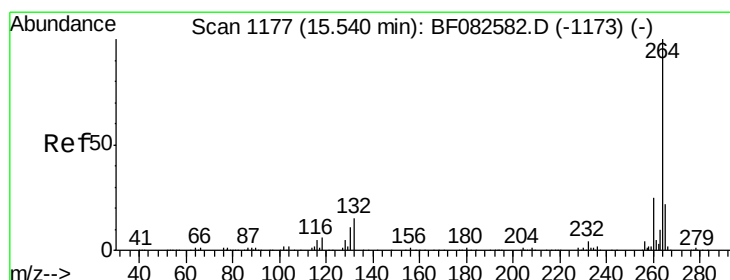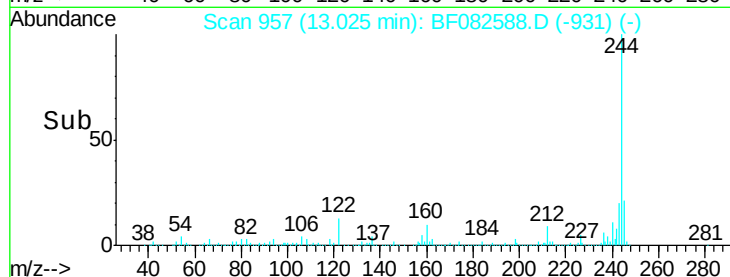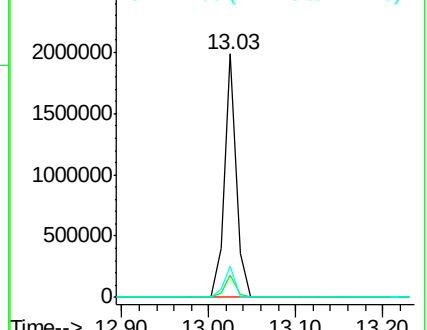

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.53 min Scan# 1176

Delta R.T. -0.01 min

Lab File: BF082588.D

Acq: 30 Oct 2015 23:00


Tgt Ion:264 Resp: 432917

Ion Ratio Lower Upper

264 100

260 24.2 19.8 29.6

265 22.2 17.4 26.0

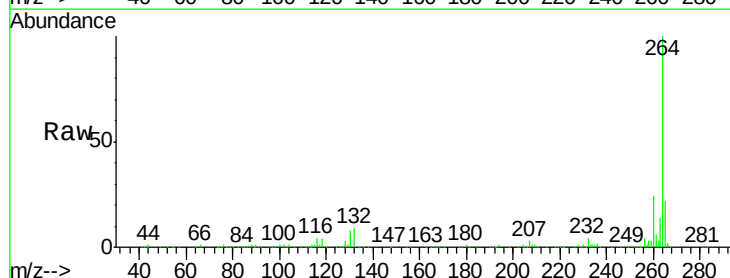

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

