

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103015\
 Data File : BF082622.D
 Acq On : 31 Oct 2015 15:34
 Operator : UM/IZ
 Sample : G4200-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T-22L

Quant Time: Nov 02 04:43:39 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 31 00:17:39 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	229620	20.00	ng	-0.01
21) Naphthalene-d8	8.19	136	942516	20.00	ng	0.00
38) Acenaphthene-d10	9.95	164	490242	20.00	ng	0.00
63) Phenanthrene-d10	11.44	188	842207	20.00	ng	0.00
75) Chrysene-d12	14.08	240	558757	20.00	ng	0.00
86) Perylene-d12	15.53	264	502583	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	1419990	93.14	ng	0.01
7) Phenol-d6	6.53	99	1632655	80.61	ng	0.00
23) Nitrobenzene-d5	7.46	82	1268433	54.96	ng	-0.01
41) 2,4,6-Tribromophenol	10.74	330	463808	86.45	ng	0.00
44) 2-Fluorobiphenyl	9.28	172	1851208	53.61	ng	0.00
78) Terphenyl-d14	13.02	244	1502535	58.85	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.66	163	524258	13.09	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103015\
Data File : BF082622.D
Acq On : 31 Oct 2015 15:34
Operator : UM/IZ
Sample : G4200-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T-22L

Quant Time: Nov 02 04:43:39 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

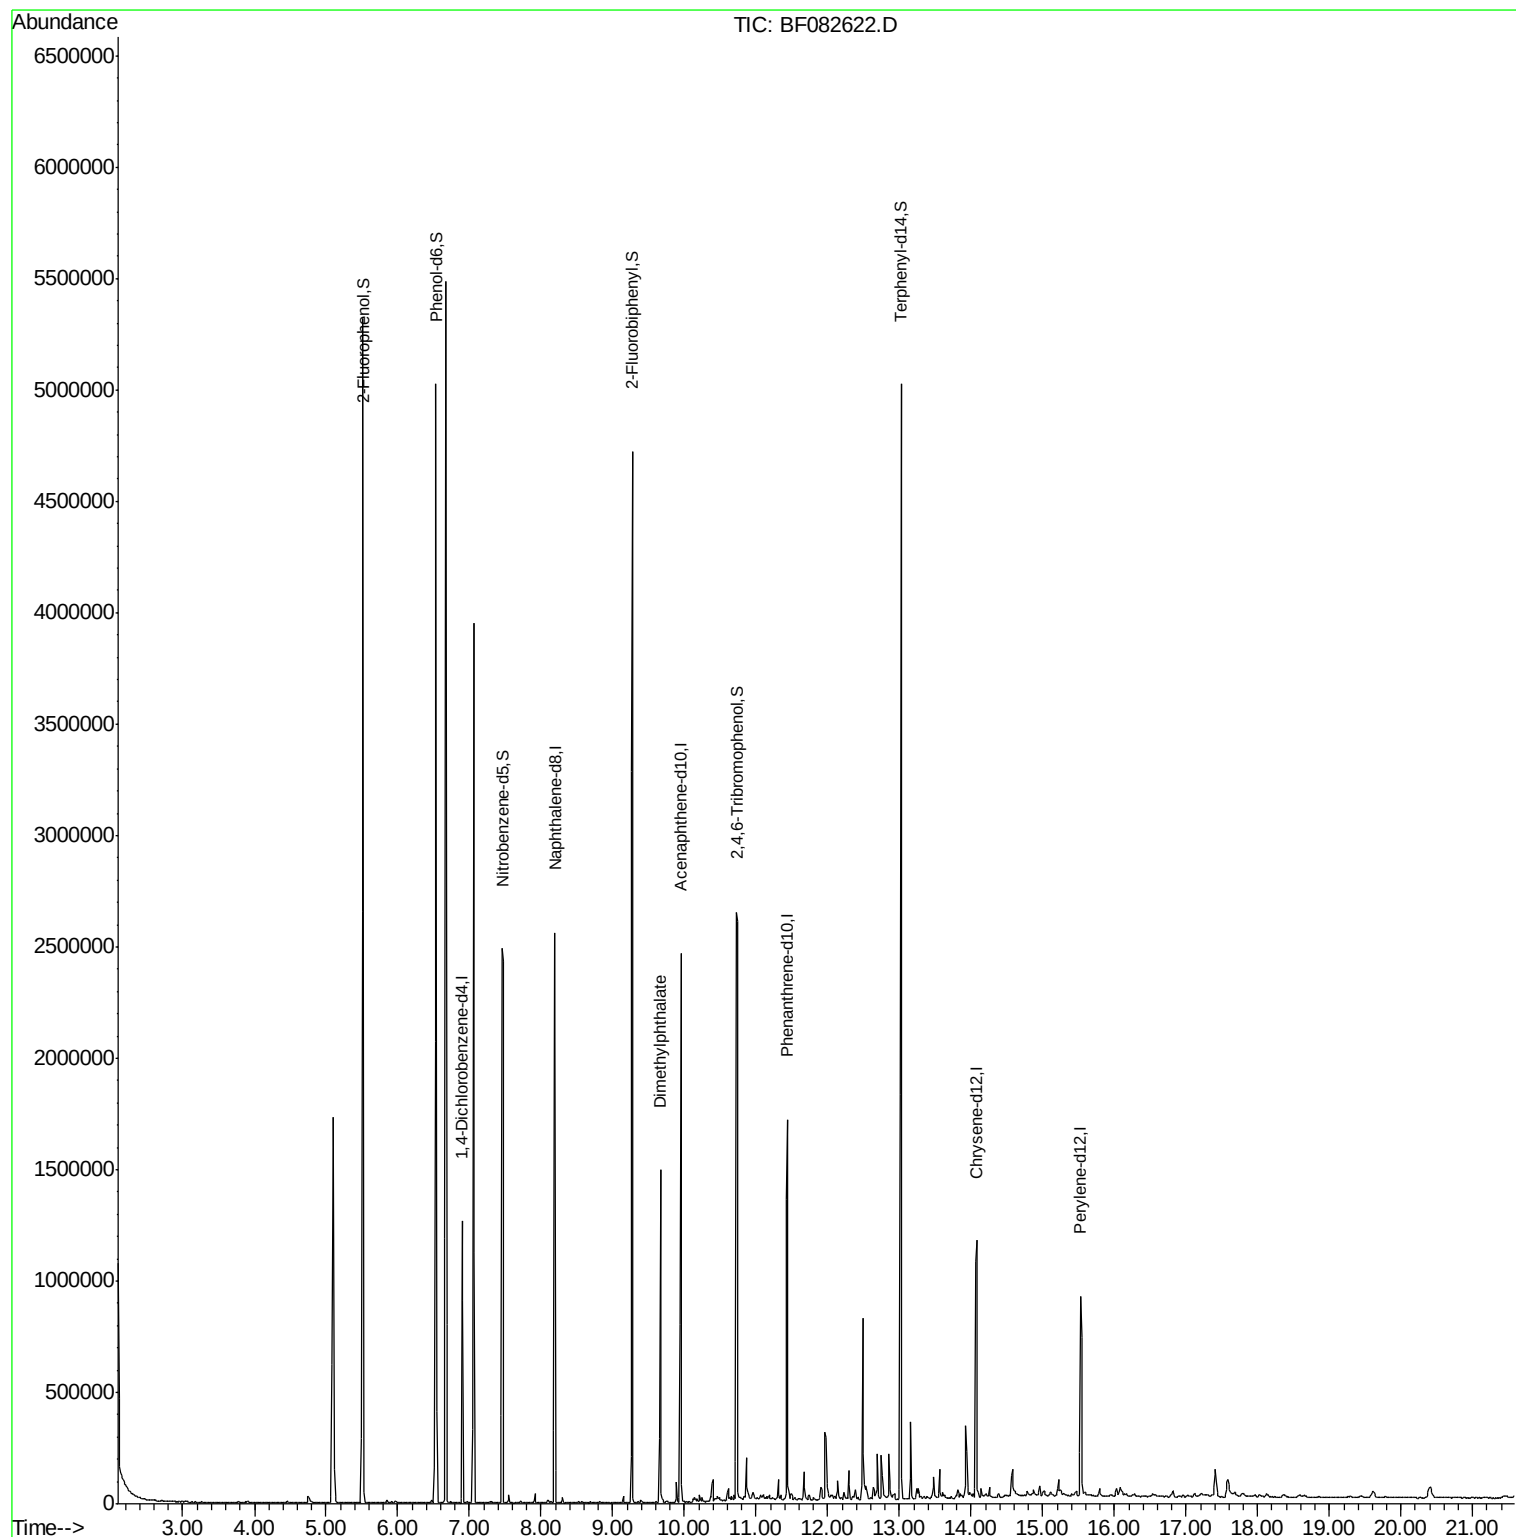

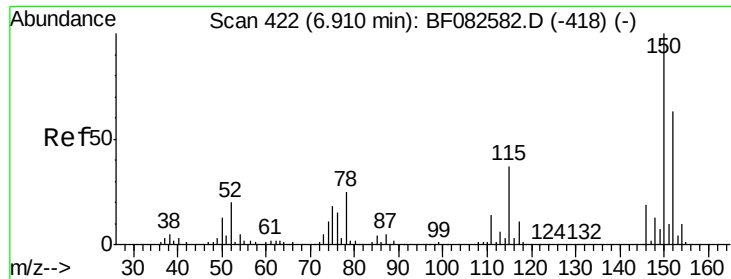


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.90 min Scan# 421
 Delta R.T. -0.01 min
 Lab File: BF082622.D
 Acq: 31 Oct 2015 15:34

Instrument :
 BNA_F
 ClientSampleId :
 T-22L

Tgt Ion:152 Resp: 229620
 Ion Ratio Lower Upper
 152 100
 150 158.4 127.0 190.4
 115 78.6 47.0 70.6#

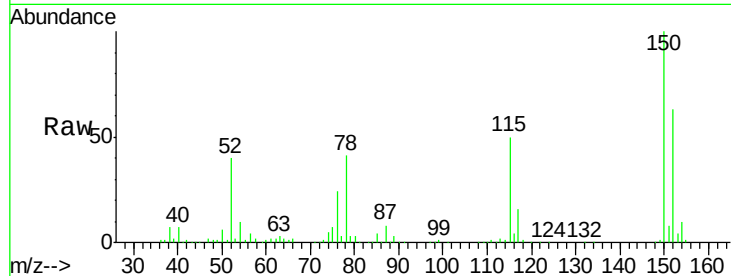


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

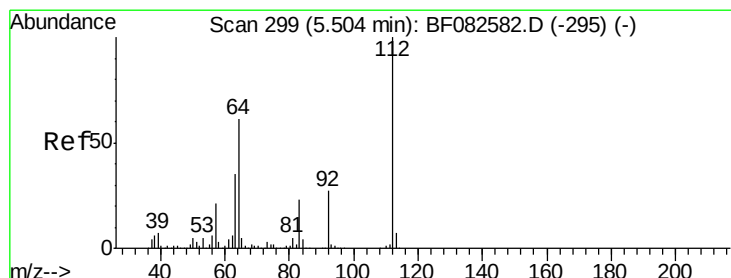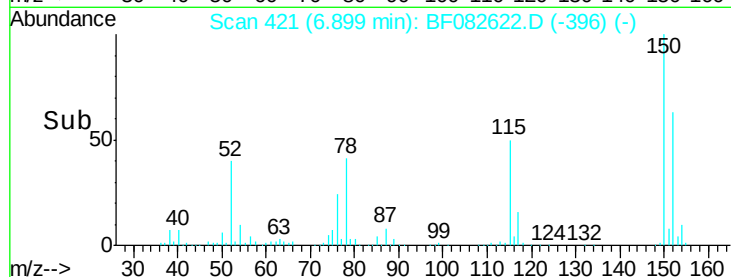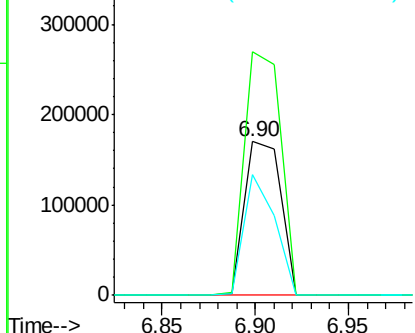



#5


2-Fluorophenol
 Concen: 93.14 ng
 RT: 5.52 min Scan# 300
 Delta R.T. 0.01 min
 Lab File: BF082622.D
 Acq: 31 Oct 2015 15:34

Tgt Ion:112 Resp: 1419990
 Ion Ratio Lower Upper
 112 100
 64 66.5 48.9 73.3
 63 37.3 28.1 42.1

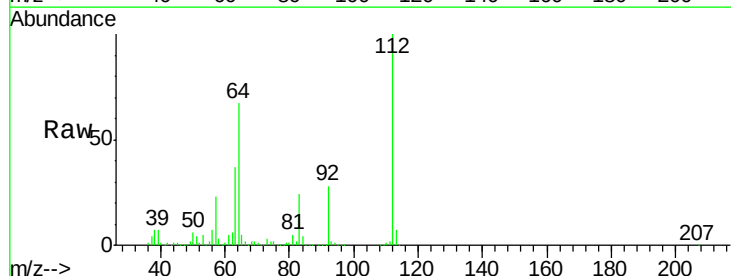

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

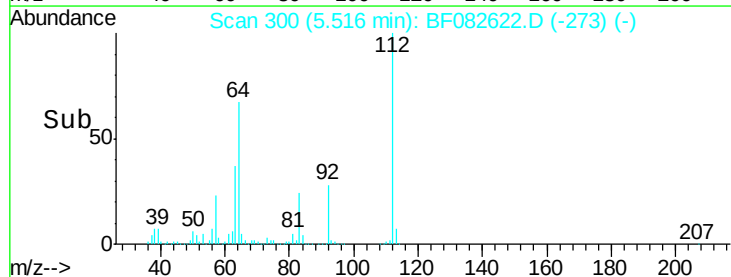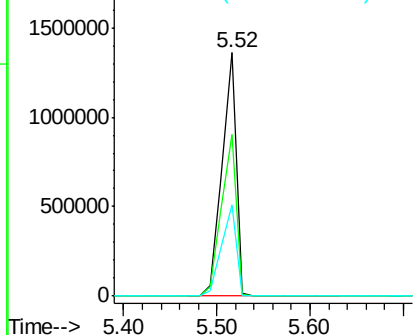

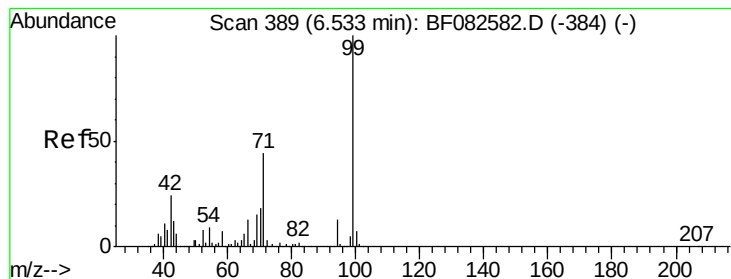

#7

Phenol-d6

Concen: 80.61 ng

RT: 6.53 min Scan# 389

Delta R.T. -0.00 min

Lab File: BF082622.D

Acq: 31 Oct 2015 15:34

Instrument :

BNA_F

ClientSampleId :

T-22L





Tgt Ion: 99 Resp: 1632655

Ion Ratio Lower Upper

99 100

42 23.7 19.2 28.8

71 44.1 35.0 52.4

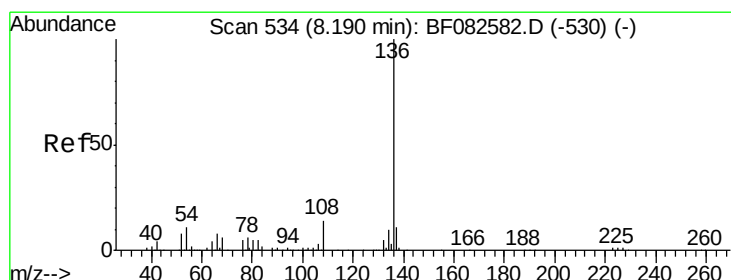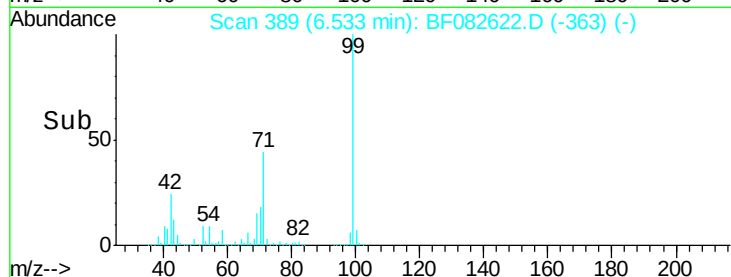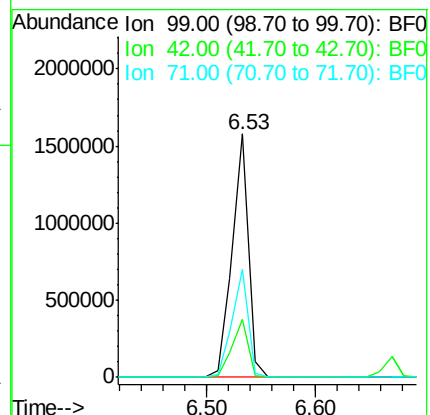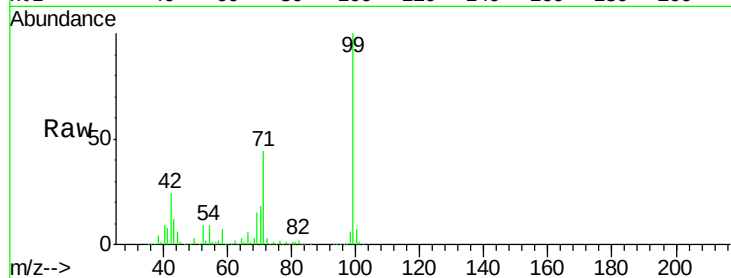

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.19 min Scan# 534

Delta R.T. -0.00 min

Lab File: BF082622.D

Acq: 31 Oct 2015 15:34

Tgt Ion: 136 Resp: 942516




Ion Ratio Lower Upper


136 100

137 11.4 9.1 13.7

54 9.5 9.1 13.7

68 5.5 4.8 7.2

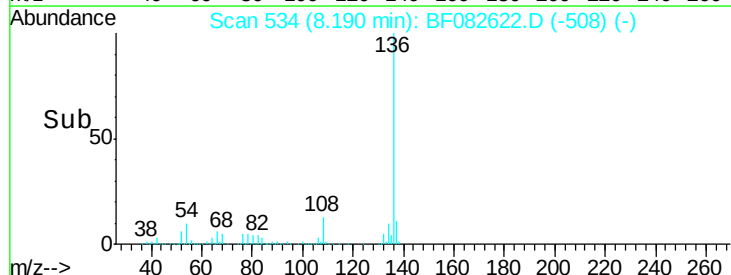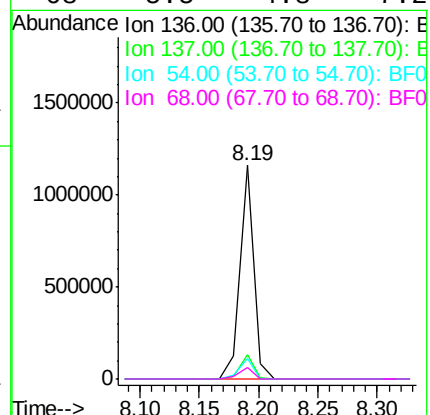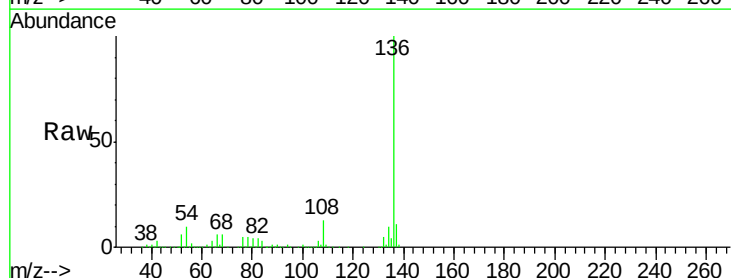


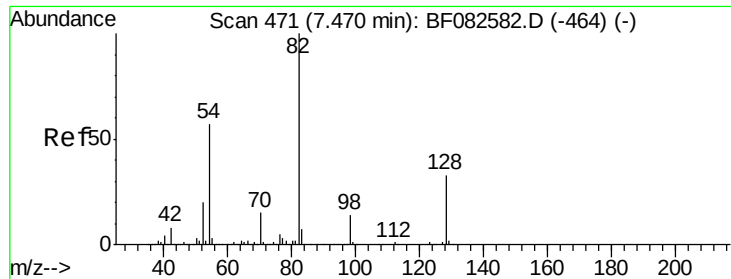




#23
 Nitrobenzene-d5
 Concen: 54.96 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.01 min
 Lab File: BF082622.D
 Acq: 31 Oct 2015 15:34

Instrument :
 BNA_F
 ClientSampleId :
 T-22L

Tgt Ion: 82 Resp: 1268433
 Ion Ratio Lower Upper
 82 100
 128 32.4 26.8 40.2
 54 57.7 45.7 68.5

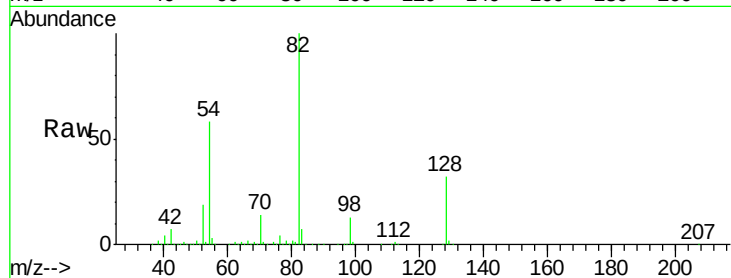


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

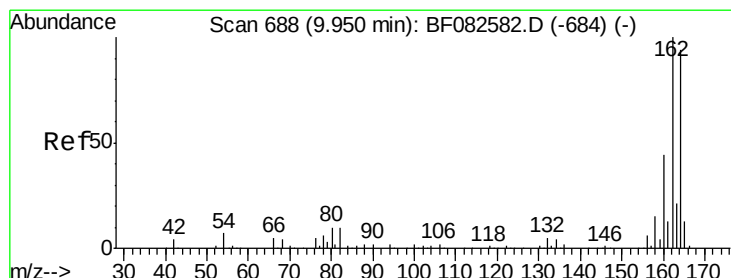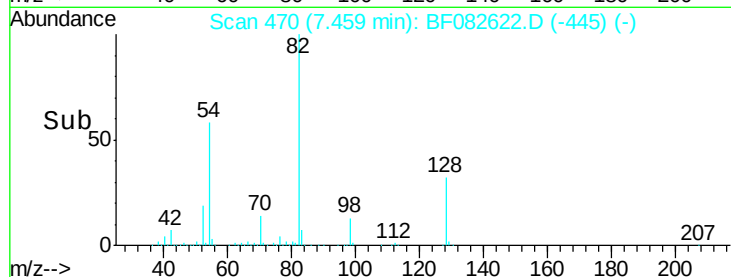
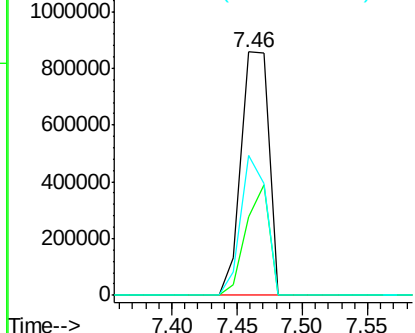



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.95 min Scan# 688
 Delta R.T. -0.00 min
 Lab File: BF082622.D
 Acq: 31 Oct 2015 15:34

Tgt Ion: 164 Resp: 490242
 Ion Ratio Lower Upper
 164 100
 162 103.4 84.9 127.3
 160 46.1 37.5 56.3

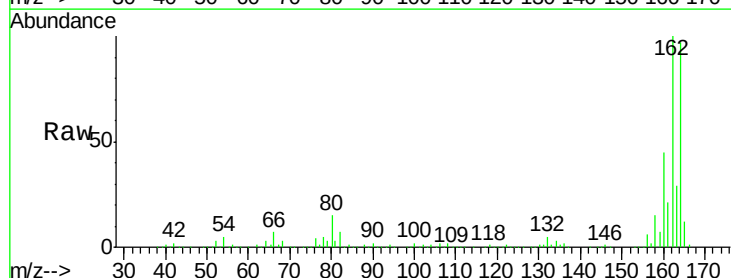

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

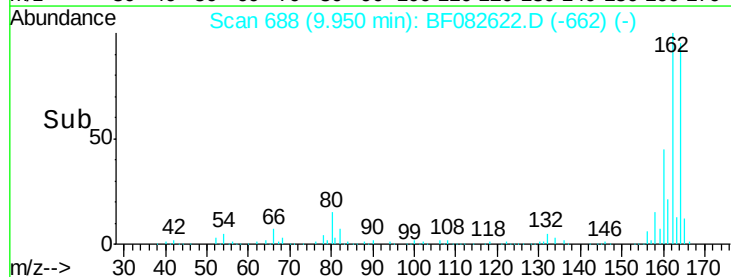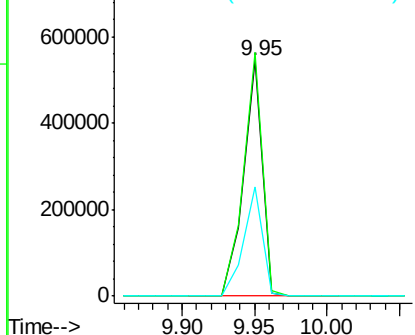


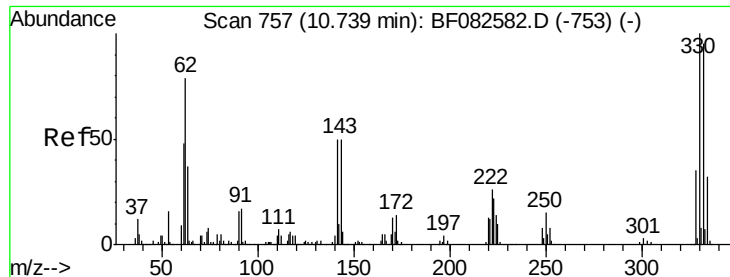




#41
 2,4,6-Tribromophenol
 Concen: 86.45 ng
 RT: 10.74 min Scan# 757
 Delta R.T. -0.00 min
 Lab File: BF082622.D
 Acq: 31 Oct 2015 15:34

Instrument :
 BNA_F
 ClientSampleId :
 T-22L

Tgt Ion:330 Resp: 463808
 Ion Ratio Lower Upper
 330 100
 332 97.9 76.6 114.8
 141 34.9 41.2 61.8#

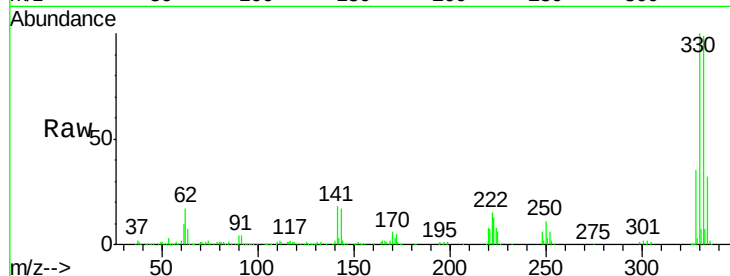


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

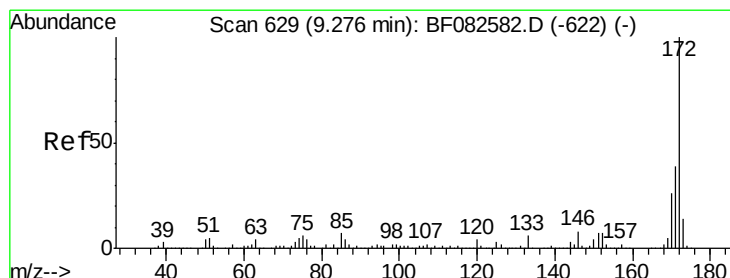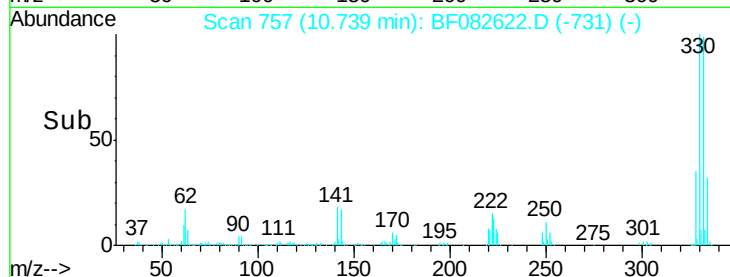
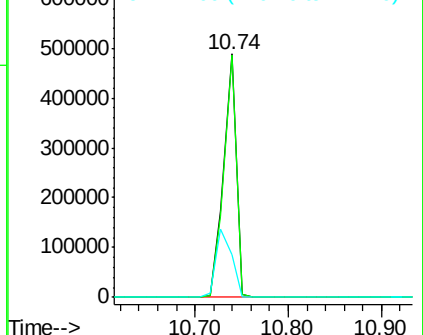



#44
 2-Fluorobiphenyl
 Concen: 53.61 ng
 RT: 9.28 min Scan# 629
 Delta R.T. -0.00 min
 Lab File: BF082622.D
 Acq: 31 Oct 2015 15:34

Tgt Ion:172 Resp: 1851208
 Ion Ratio Lower Upper
 172 100
 171 37.3 30.8 46.2
 170 25.3 21.2 31.8

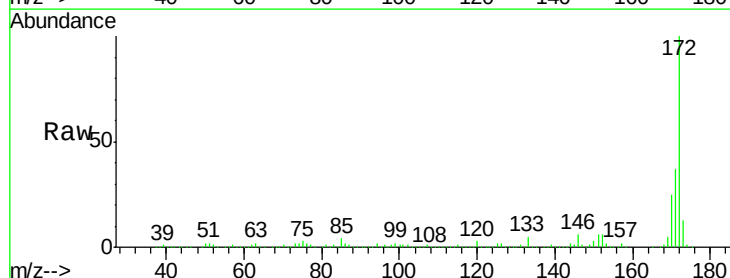

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

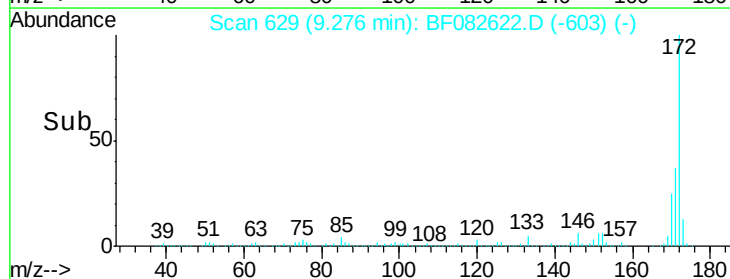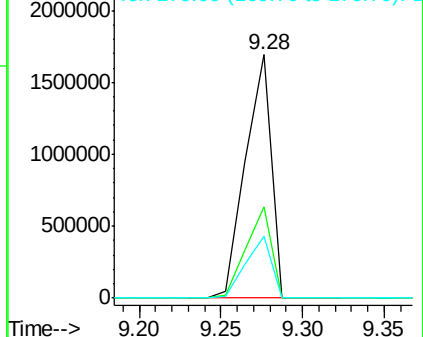

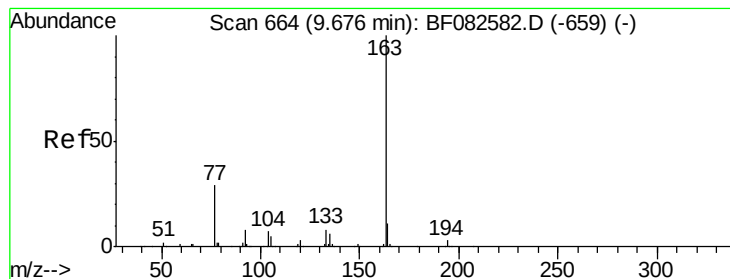

#49

Dimethylphthalate

Concen: 13.09 ng

RT: 9.66 min Scan# 663

Delta R.T. -0.01 min

Lab File: BF082622.D

Acq: 31 Oct 2015 15:34

Instrument :

BNA_F

ClientSampleId :

T-22L


Tgt Ion:163 Resp: 524258

Ion Ratio Lower Upper

163 100

194 3.6 2.6 4.0




164 10.4 8.7 13.1

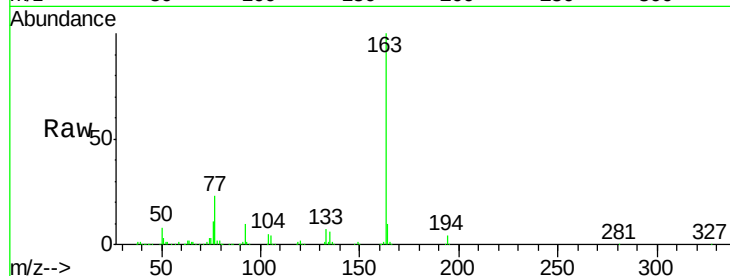

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

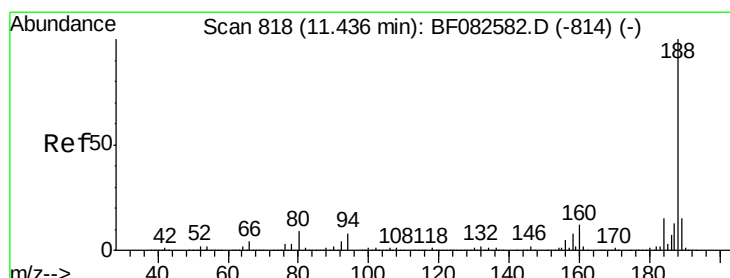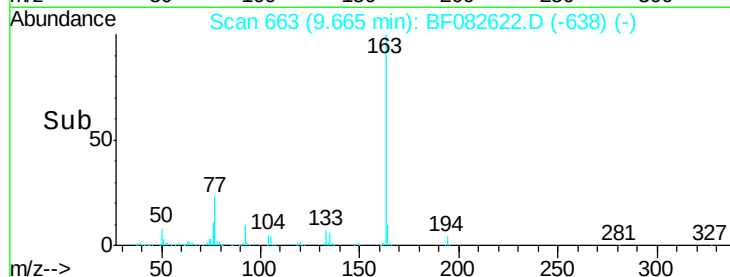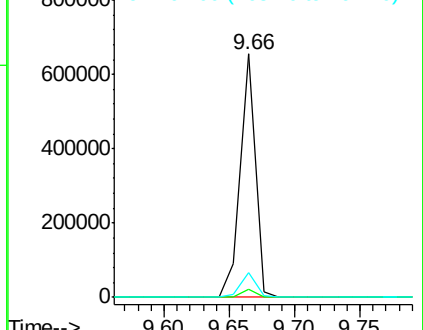

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.44 min Scan# 818

Delta R.T. -0.00 min

Lab File: BF082622.D

Acq: 31 Oct 2015 15:34


Tgt Ion:188 Resp: 842207

Ion Ratio Lower Upper

188 100

94 5.2 6.1 9.1#



80 5.6 7.0 10.6#

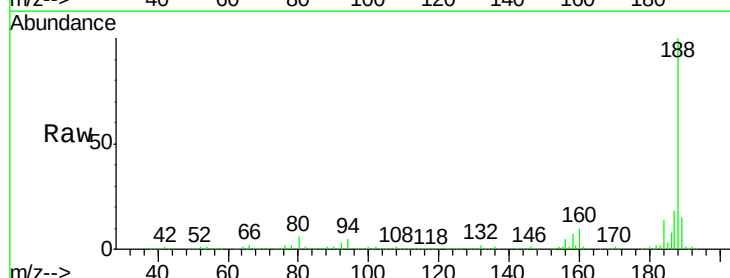


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

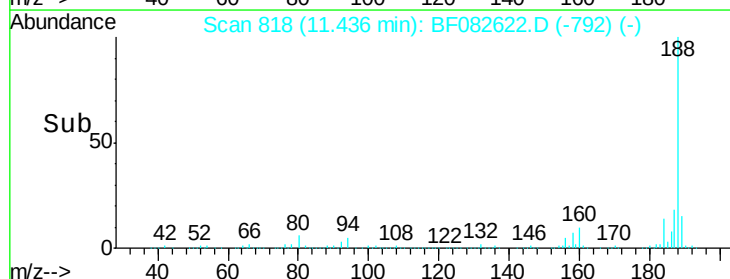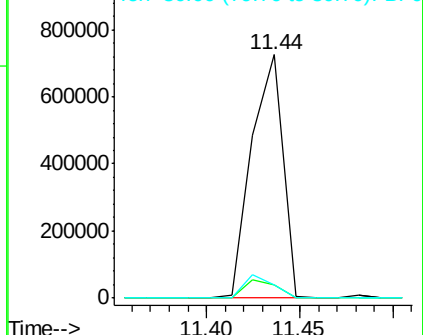

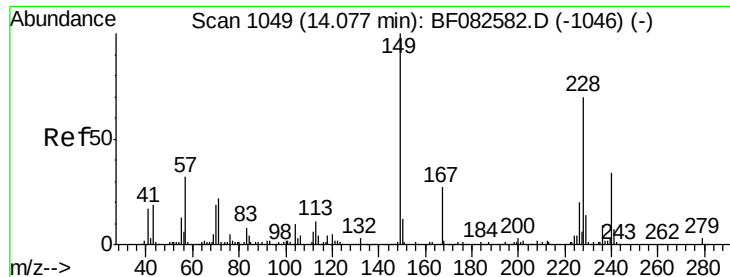

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.08 min Scan# 1049

Delta R.T. -0.00 min

Lab File: BF082622.D

Acq: 31 Oct 2015 15:34

Instrument :

BNA_F

ClientSampleId :

T-22L


Tgt Ion:240 Resp: 558757

Ion Ratio Lower Upper

240 100

120 4.3 10.9 16.3#

236 25.9 21.6 32.4

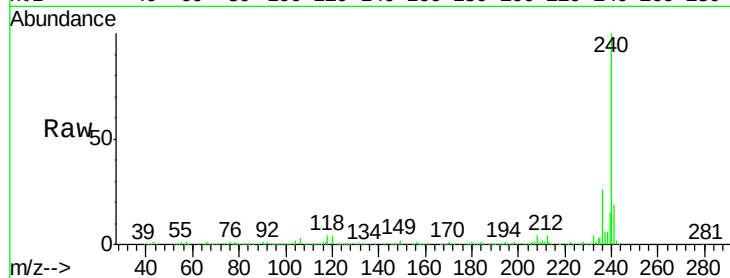

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

600000

500000

400000

300000

200000

100000



0

14.00

14.10

14.20

Time-->

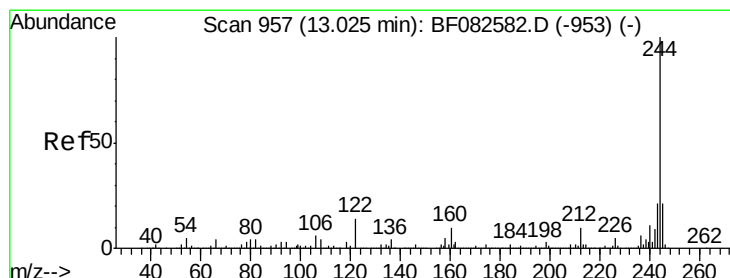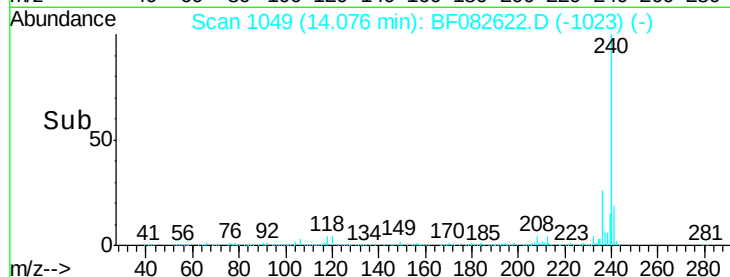

#78

Terphenyl-d14

Concen: 58.85 ng

RT: 13.02 min Scan# 957

Delta R.T. -0.00 min

Lab File: BF082622.D

Acq: 31 Oct 2015 15:34


Tgt Ion:244 Resp: 1502535

Ion Ratio Lower Upper

244 100

212 8.8 7.6 11.4

122 8.7 11.3 16.9#

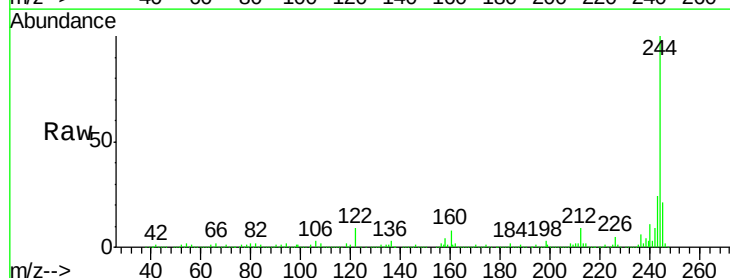

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

2000000

1500000

1000000

500000


0


12.90

13.00

13.10

Time-->

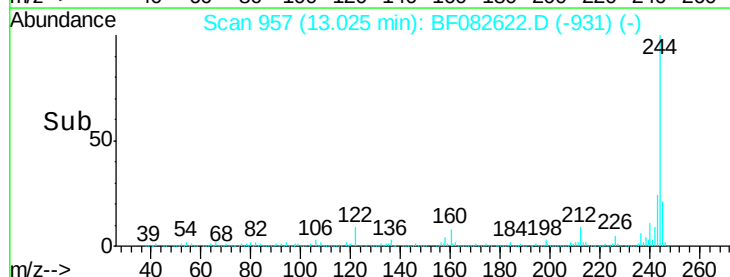


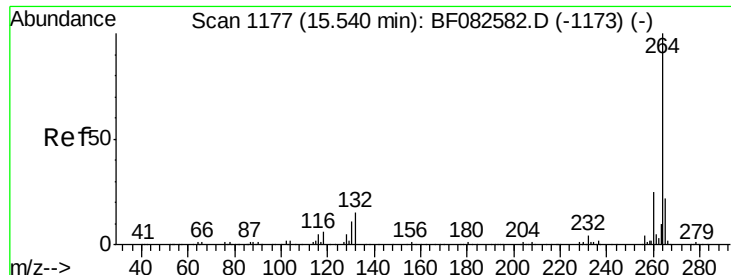

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.53 min Scan# 1176
Delta R.T. -0.01 min
Lab File: BF082622.D
Acq: 31 Oct 2015 15:34

Instrument :
BNA_F
ClientSampleId :
T-22L

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.8	29.6
265	21.7	17.4	26.0

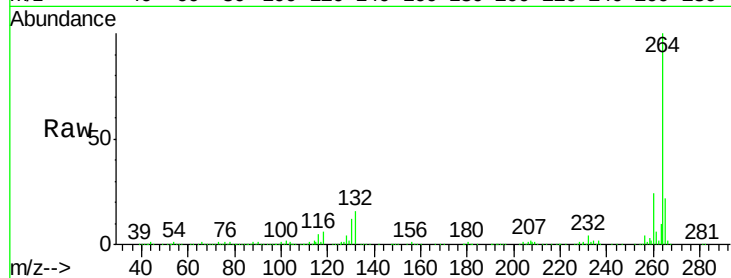

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

