


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF103015\  
Data File : BF082578.D  
Acq On : 30 Oct 2015 17:36  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF103015.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sat Oct 31 00:17:39 2015

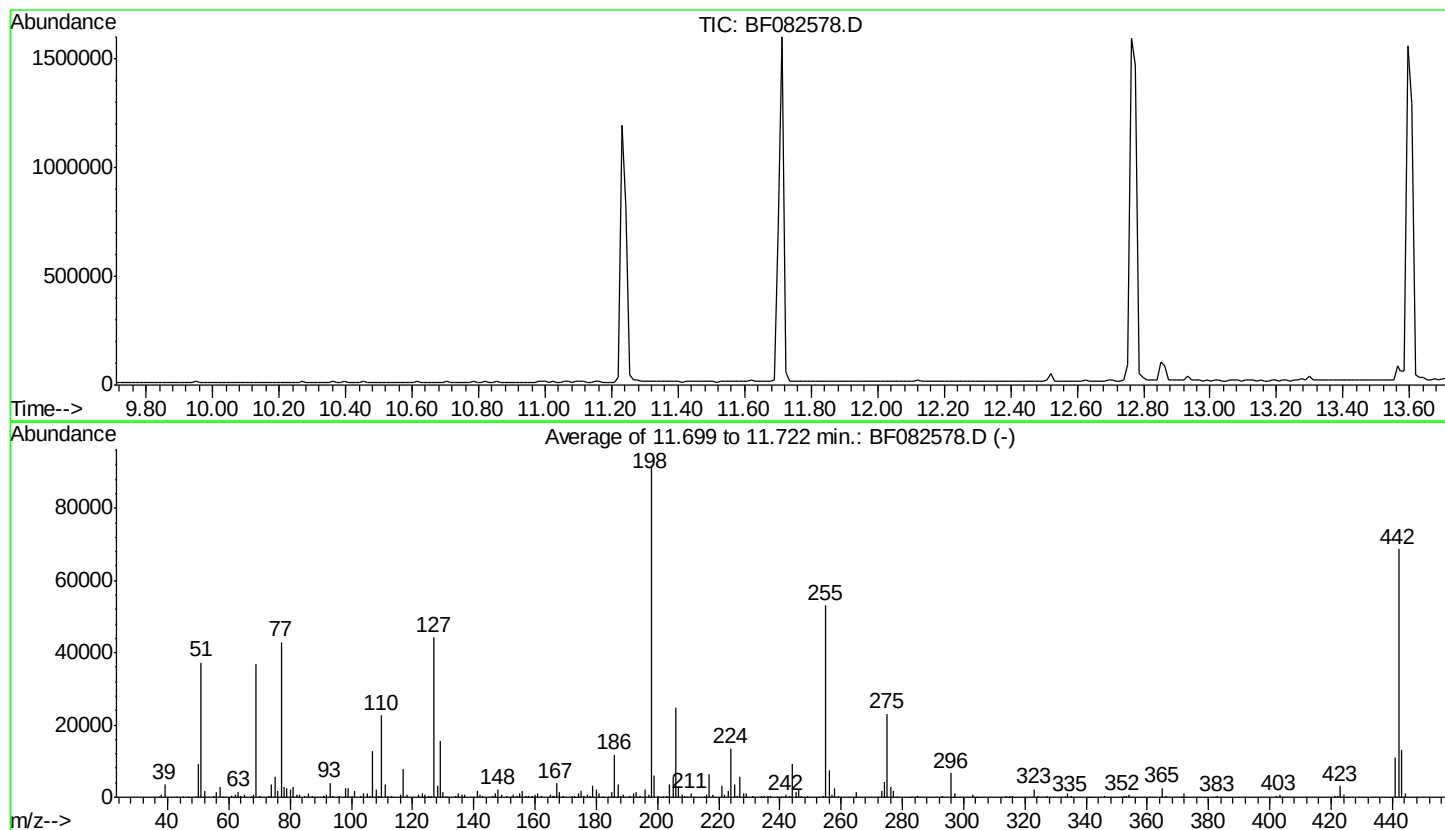

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 837

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.6      | 37244   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 603     | PASS             |
| 69          | 198          | 0.00         | 100          | 40.2      | 36901   | PASS             |
| 70          | 69           | 0.00         | 2            | 1.0       | 354     | PASS             |
| 127         | 198          | 10           | 80           | 48.1      | 44147   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 623     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 91815   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 6112    | PASS             |
| 275         | 198          | 10           | 60           | 25.2      | 23139   | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 2652    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.8      | 10826   | PASS             |
| 442         | 198          | 50           | 100          | 74.7      | 68609   | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 13263   | PASS             |