


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103015\
 Data File : BF082601.D
 Acq On : 31 Oct 2015 5:24
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 31 00:17:39 2015

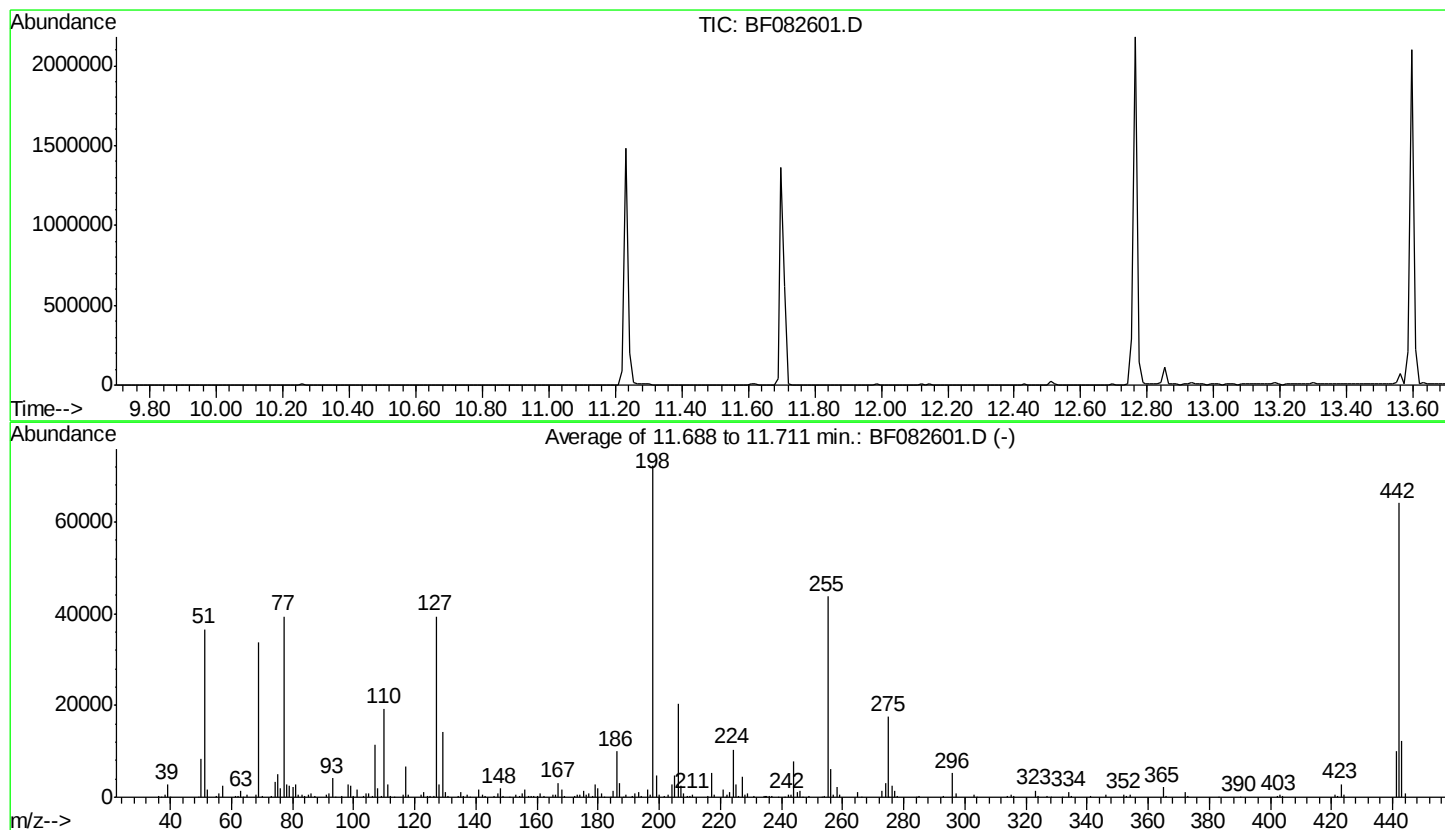

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	36584	PASS
68	69	0.00	2	1.4	473	PASS
69	198	0.00	100	46.8	33857	PASS
70	69	0.00	2	0.4	152	PASS
127	198	10	80	54.4	39340	PASS
197	198	0.00	2	0.9	651	PASS
198	198	100	100	100.0	72268	PASS
199	198	5	9	6.6	4738	PASS
275	198	10	60	24.2	17480	PASS
365	198	1	100	3.1	2225	PASS
441	442	0.01	24	15.5	9923	PASS
442	198	50	100	88.8	64138	PASS
443	442	15	24	19.2	12306	PASS