
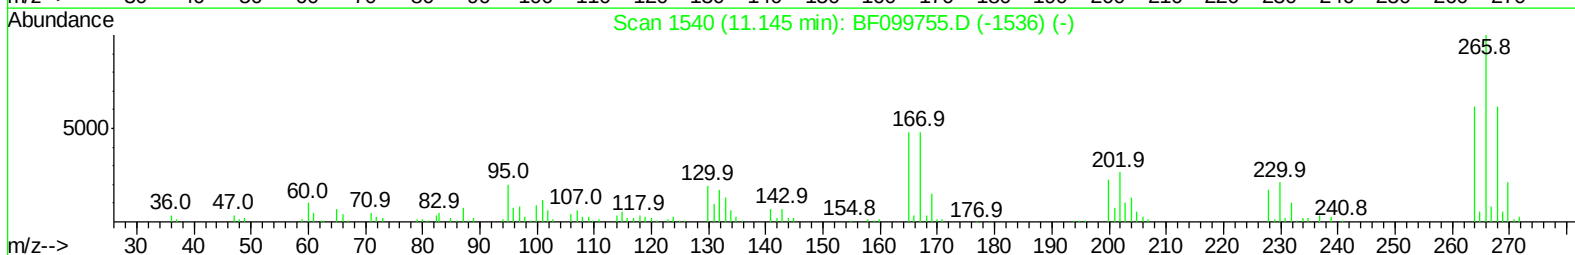
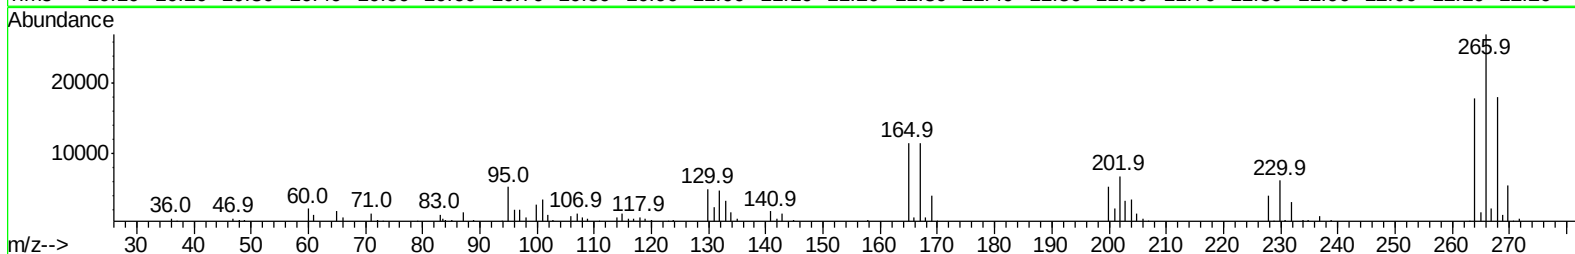


Data Path : Z:\HPCHEM1\BNA F\DATA\BF103017\
Data File : BF099950.D
Acq On : 30 Oct 2017 11:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 04:46:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 27 15:58:57 2017
Response via : Initial Calibration

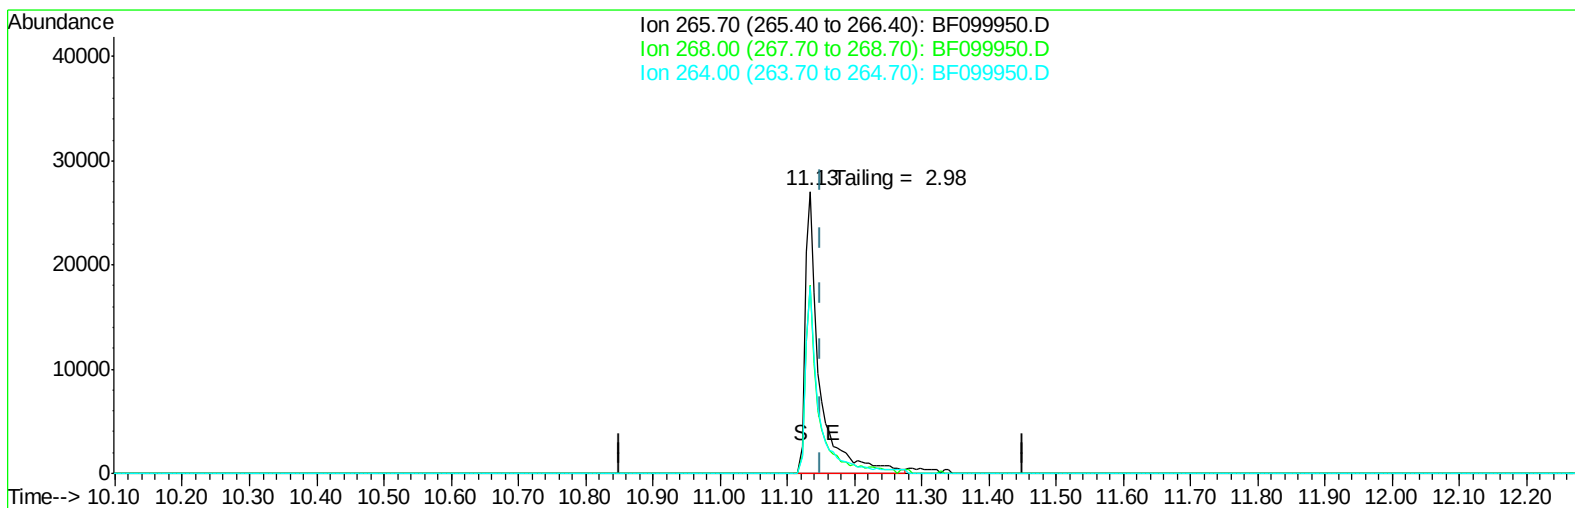

TIC: BF099950.D

(69) Pentachlorophenol (C)




11.133min (-0.018) 65252.93ng

response 40541

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.05
264.00	61.90	66.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF103017\
Data File : BF099950.D
Acq On : 30 Oct 2017 11:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 04:46:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 27 15:58:57 2017
Response via : Initial Calibration

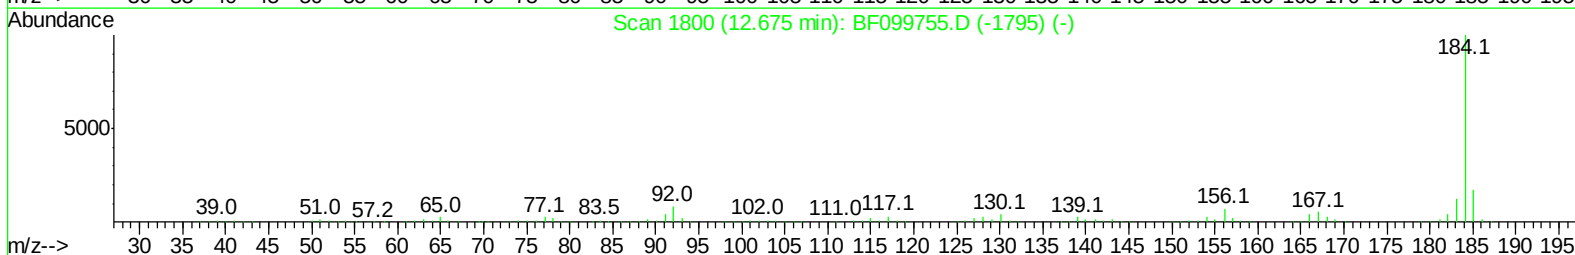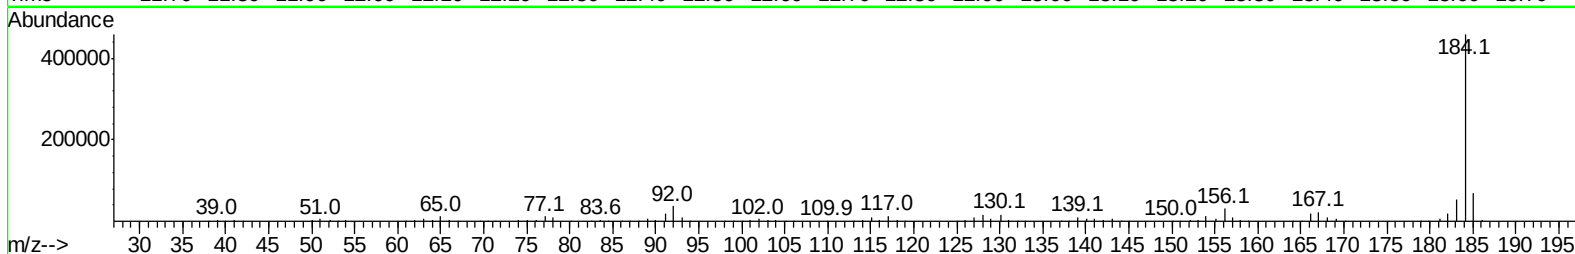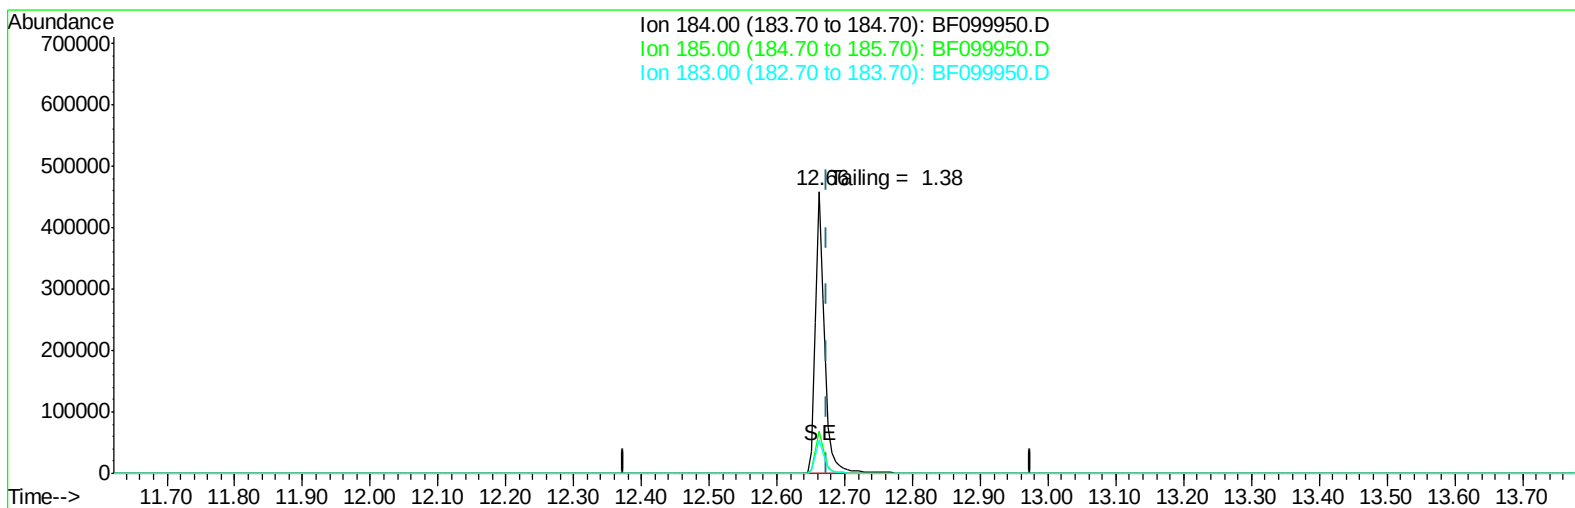

TIC: BF099950.D

(76) Benzidine

12.663min (-0.012) 0.00ng

response 426068

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.22
183.00	11.60	11.93
0.00	0.00	0.00