


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103017\
 Data File : BF099950.D
 Acq On : 30 Oct 2017 11:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

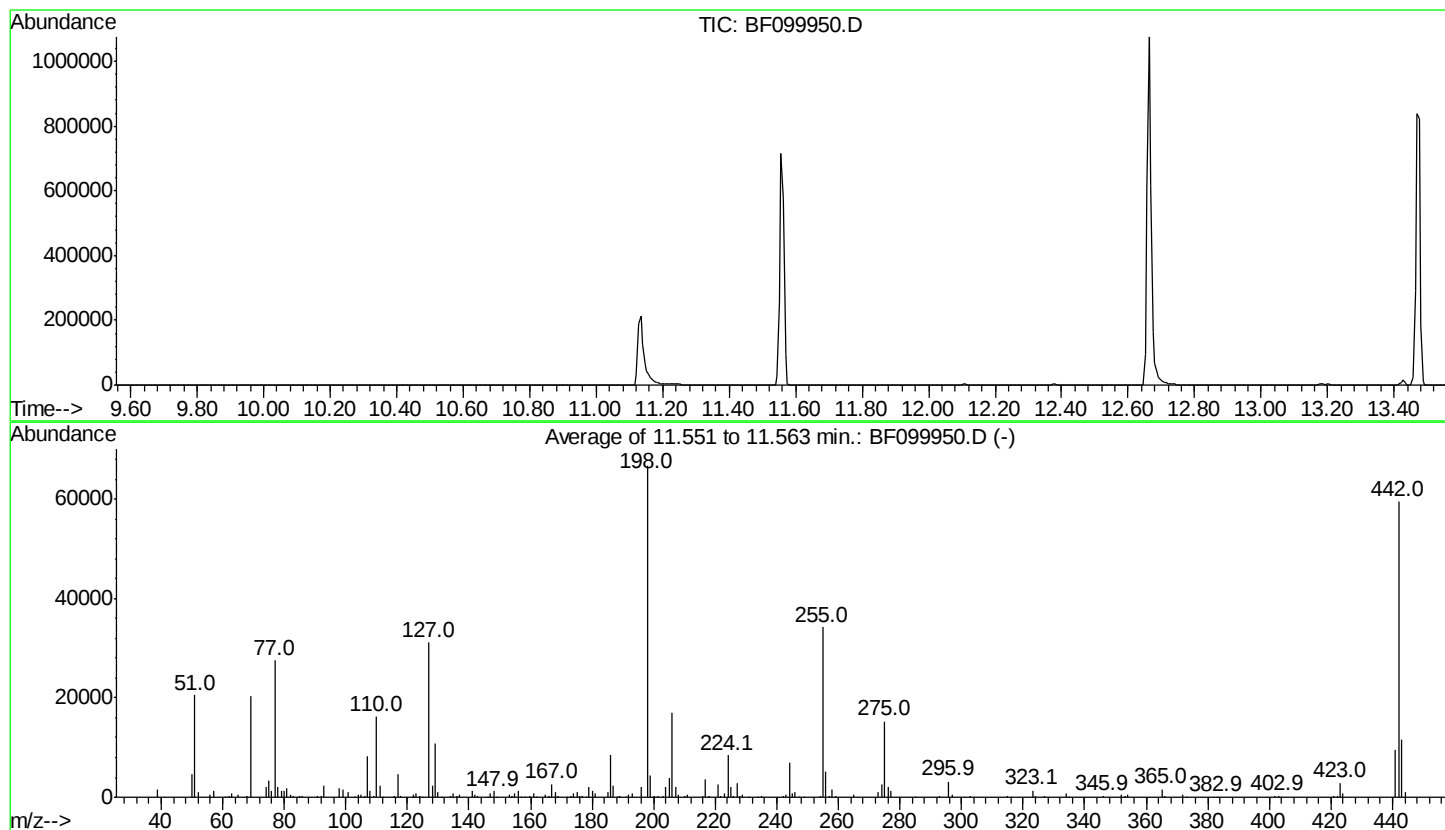

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	20599	PASS
68	69	0.00	2	0.8	154	PASS
69	198	0.00	100	30.6	20411	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	31154	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66784	PASS
199	198	5	9	6.7	4504	PASS
275	198	10	60	22.9	15311	PASS
365	198	1	100	2.4	1617	PASS
441	443	0.01	100	81.7	9443	PASS
442	198	50	100	89.0	59463	PASS
443	442	15	24	19.4	11559	PASS