


Data Path : Z:\HPCHEM1\BNA F\DATA\BF103017\
 Data File : BF099976.D
 Acq On : 30 Oct 2017 23:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

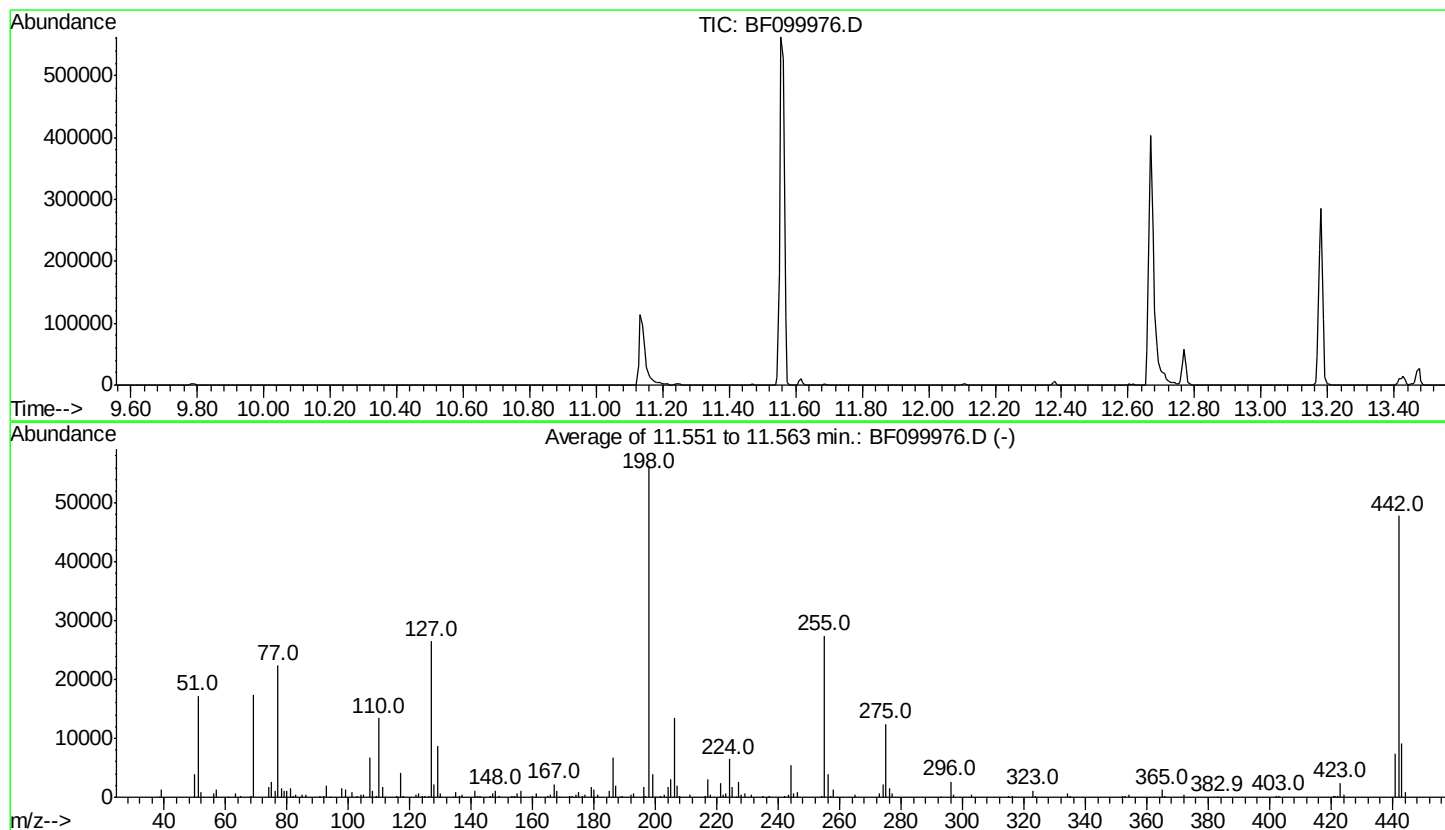

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	17237	PASS
68	69	0.00	2	1.6	279	PASS
69	198	0.00	100	30.7	17317	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	26463	PASS
197	198	0.00	2	0.4	243	PASS
198	198	100	100	100.0	56333	PASS
199	198	5	9	6.9	3911	PASS
275	198	10	60	22.1	12443	PASS
365	198	1	100	2.3	1291	PASS
441	443	0.01	100	82.5	7458	PASS
442	198	50	100	84.9	47814	PASS
443	442	15	24	18.9	9036	PASS