

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103019\
 Data File : BF117643.D
 Acq On : 31 Oct 2019 4:01
 Operator : JU
 Sample : K5582-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NCQ-632

Quant Time: Oct 31 08:14:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	34428	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	131625	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	61649	20.00	ng	-0.01
64) Phenanthrene-d10	11.25	188	92420	20.00	ng	0.00
76) Chrysene-d12	13.90	240	69385	20.00	ng	0.00
87) Perylene-d12	15.34	264	54297	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	123488	53.36	ng	0.00
7) Phenol-d6	6.39	99	112611	36.23	ng	0.01
23) Nitrobenzene-d5	7.29	82	213651	80.13	ng	-0.01
42) 2,4,6-Tribromophenol	10.56	330	38809	72.75	ng	0.00
45) 2-Fluorobiphenyl	9.08	172	356927	81.58	ng	-0.01
79) Terphenyl-d14	12.83	244	306599	72.08	ng	0.00
Target Compounds						
10) Phenol	6.41	94	16028	5.052	ng	81
50) Dimethylphthalate	9.48	163	53298	12.127	ng	# 99
74) Di-n-butylphthalate	11.80	149	37317	5.550	ng	99
80) Butylbenzylphthalate	13.30	149	10883	3.670	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103019\
Data File : BF117643.D
Acq On : 31 Oct 2019 4:01
Operator : JU
Sample : K5582-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NCQ-632

Quant Time: Oct 31 08:14:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

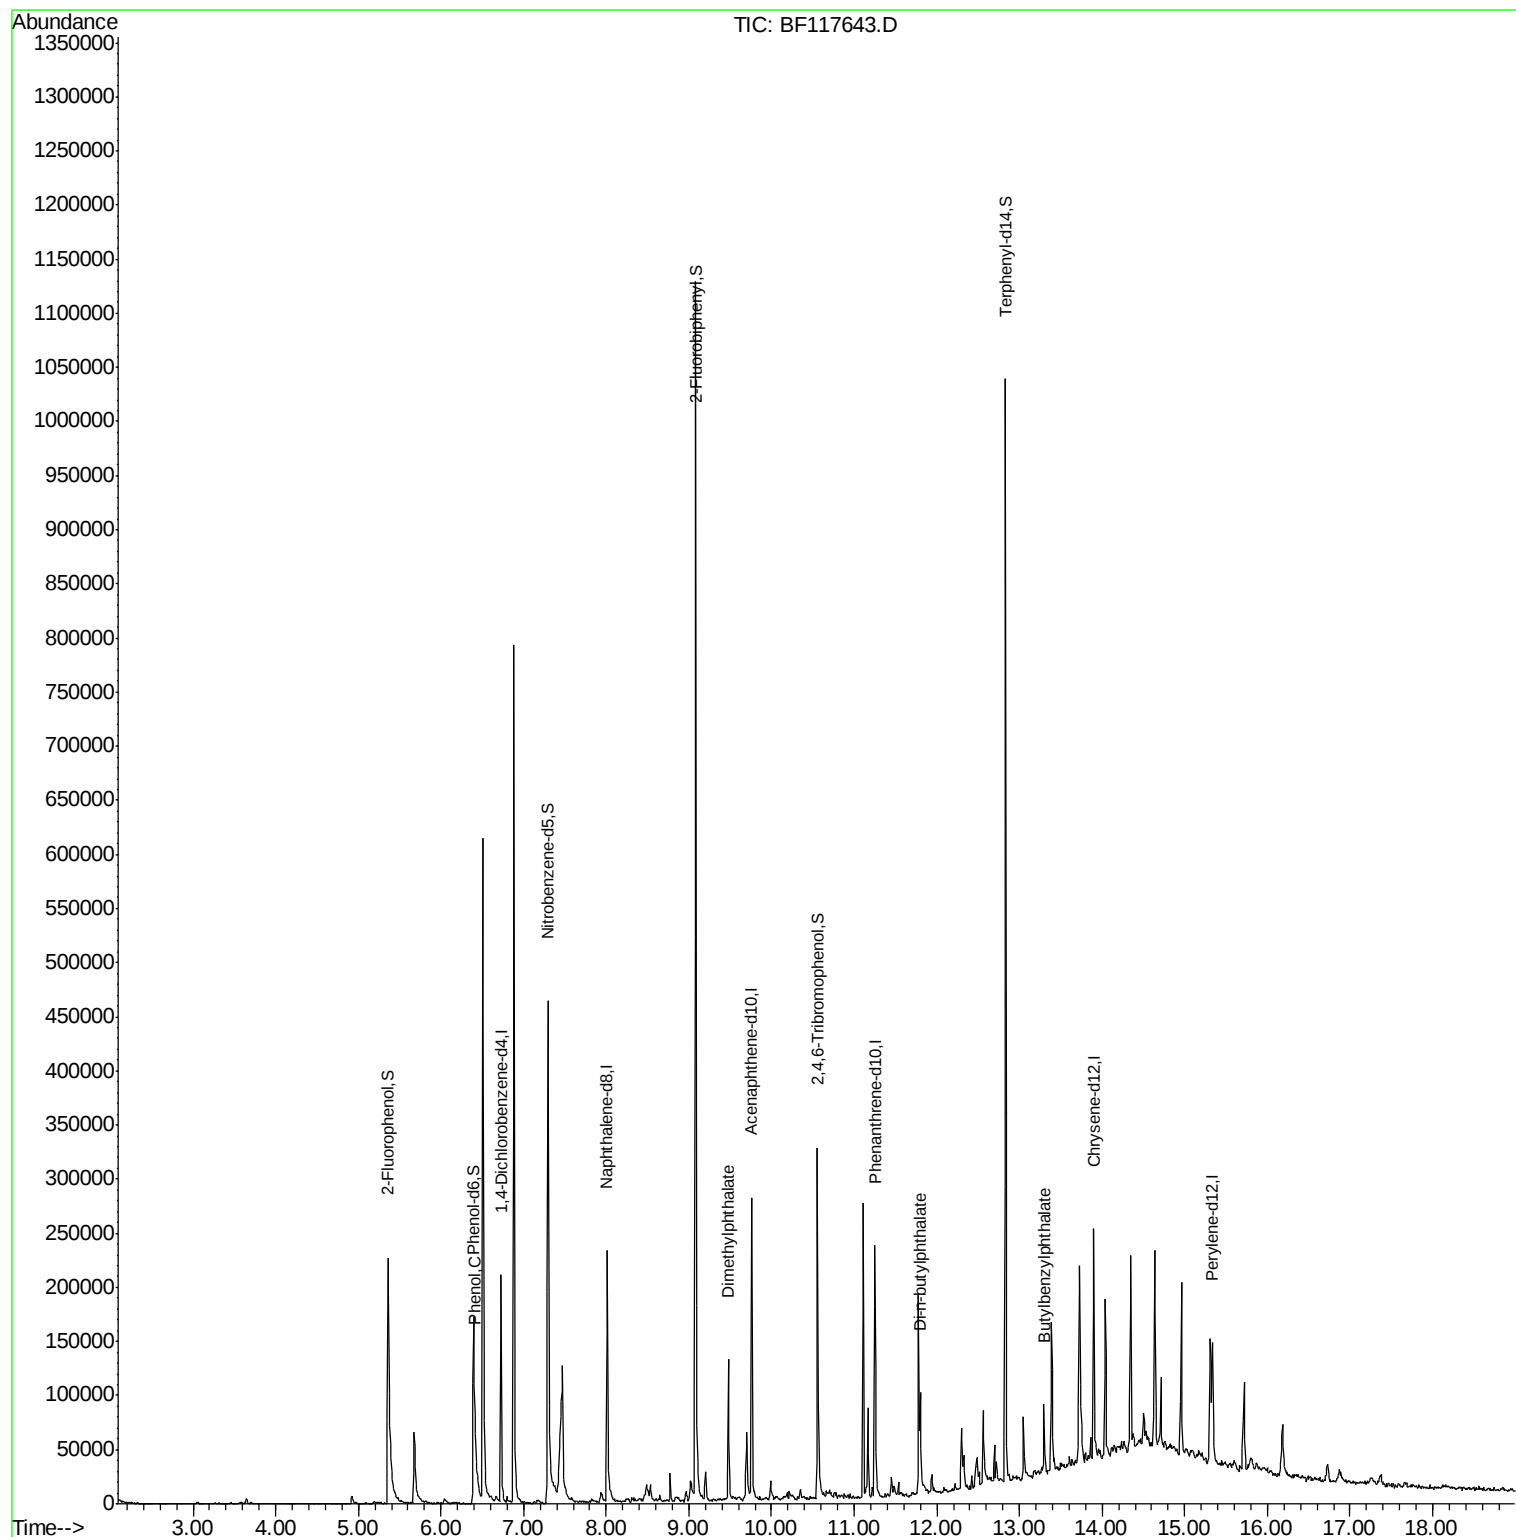




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Instrument :
BNA_F
ClientSampleId :
NCQ-632

Tot Ion:152 Resp: 34428
Ion Ratio Lower Upper
152 100
150 154.7 126.8 190.2
115 59.8 51.6 77.4

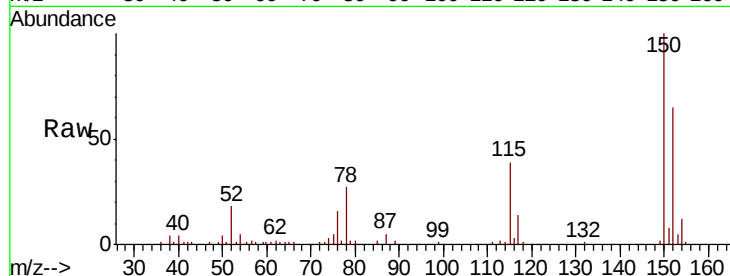


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

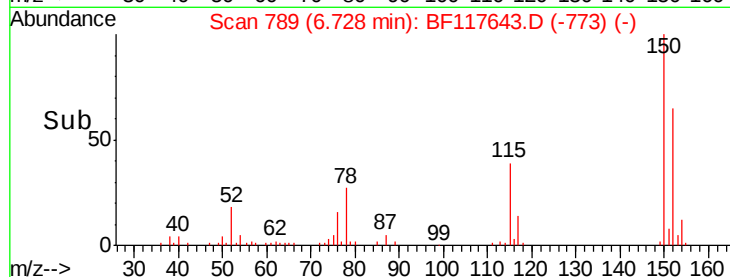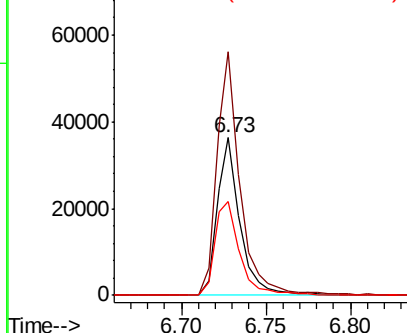



#5

2-Fluorophenol
Concen: 53.362 ng
RT: 5.36 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Tgt Ion:112 Resp: 123488
Ion Ratio Lower Upper
112 100
64 57.3 44.1 66.1
63 29.5 23.4 35.2

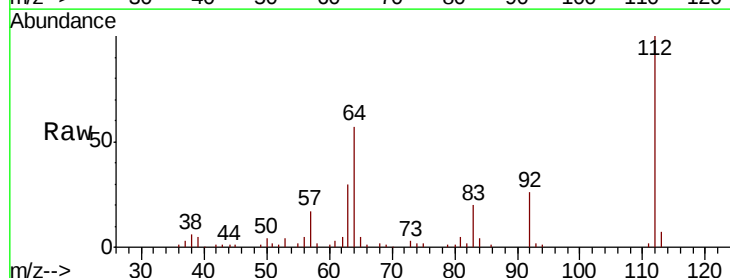

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

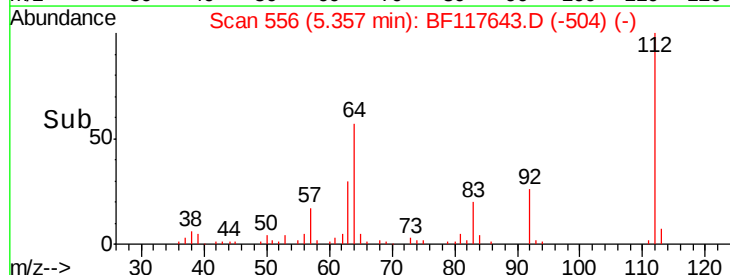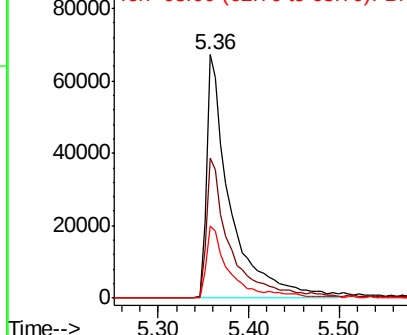



#7

Phenol-d6

Concen: 36.230 ng

RT: 6.39 min Scan# 732

Delta R.T. 0.01 min

Lab File: BF117643.D

Acq: 31 Oct 2019 4:01

Instrument :

BNA_F

ClientSampleId :

NCQ-632


Tot Ion: 99 Resp: 112611

Ion Ratio Lower Upper

99 100

42 15.9 12.8 19.2




71 36.0 28.6 43.0

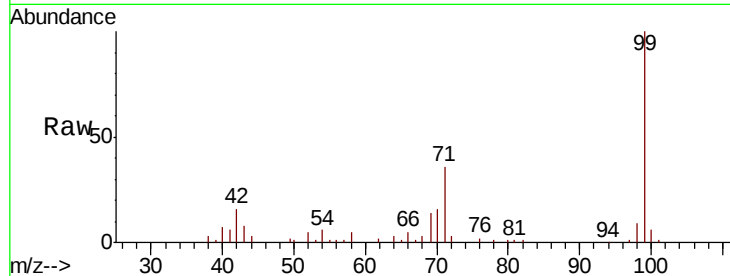

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

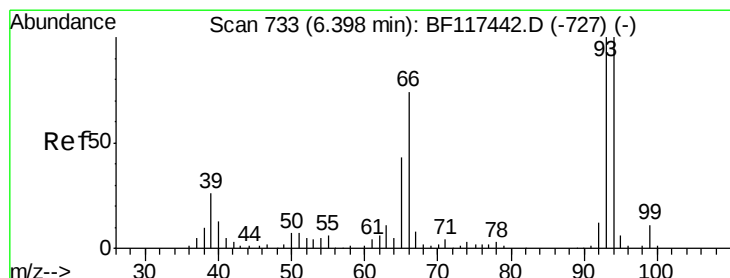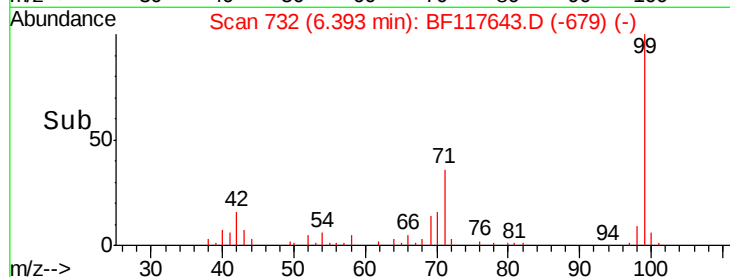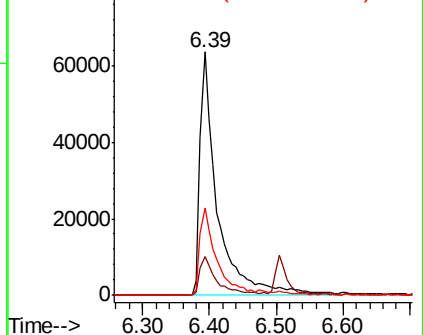

#10

Phenol

Concen: 5.052 ng

RT: 6.41 min Scan# 735

Delta R.T. 0.01 min

Lab File: BF117643.D

Acq: 31 Oct 2019 4:01


Tgt Ion: 94 Resp: 16028

Ion Ratio Lower Upper

94 100

65 30.5 23.4 63.4



66 59.3 54.7 94.7

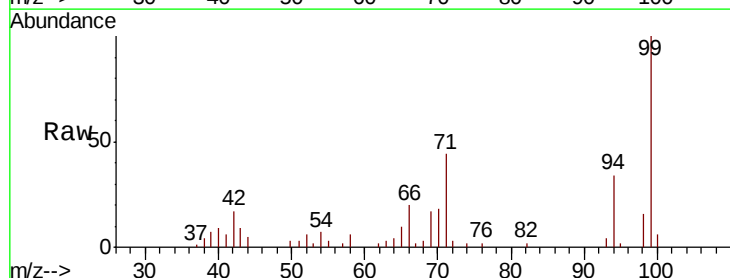


Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

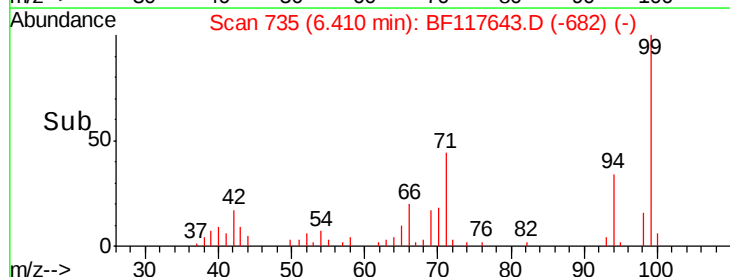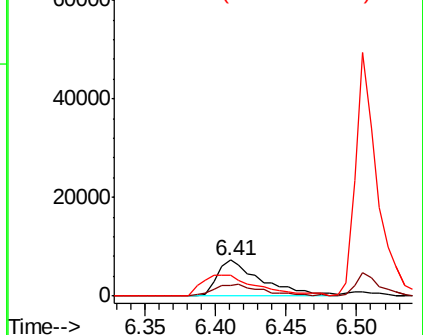


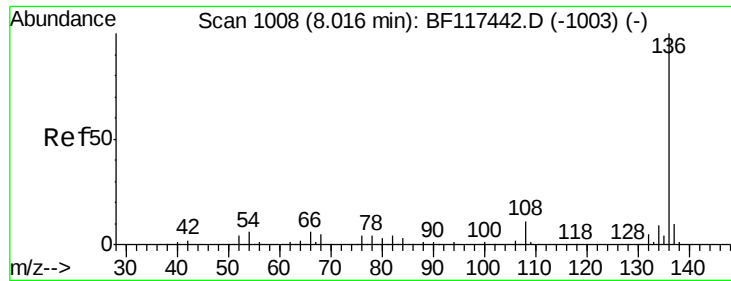




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.01 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Instrument :
BNA_F
ClientSampleId :
NCQ-632

Tot Ion:136	Resp:	131625
Ion Ratio	Lower	Upper
136	100	
137	11.2	8.2 12.4
54	6.1	4.5 6.7
68	5.6	4.3 6.5

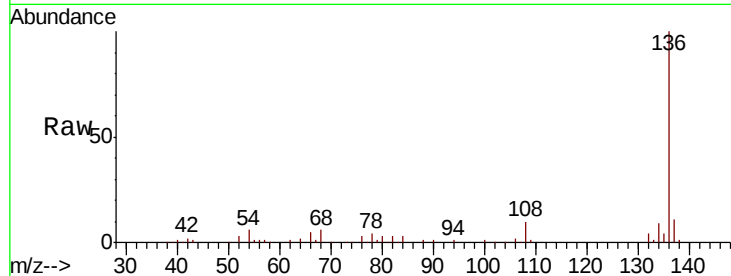


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

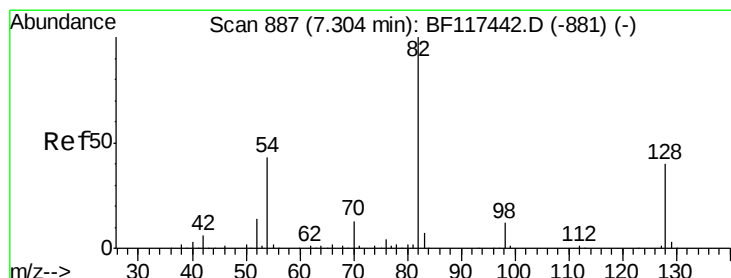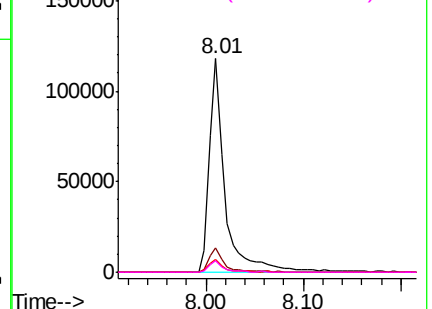
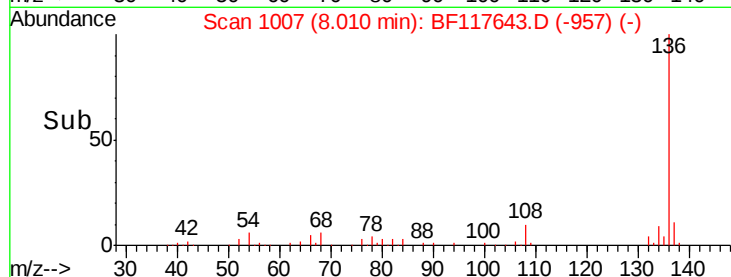



#23
Nitrobenzene-d5
Concen: 80.133 ng
RT: 7.29 min Scan# 885
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Tgt Ion: 82	Resp:	213651
Ion Ratio	Lower	Upper
82	100	
128	40.1	32.2 48.2
54	43.0	34.2 51.2

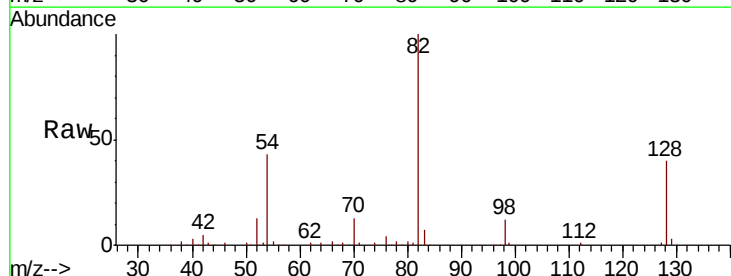

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

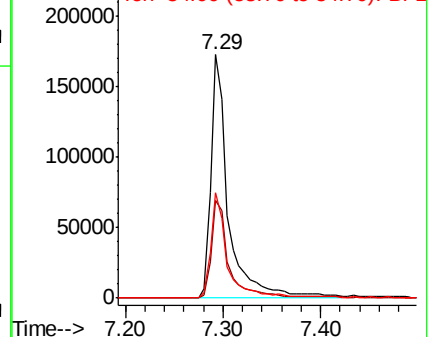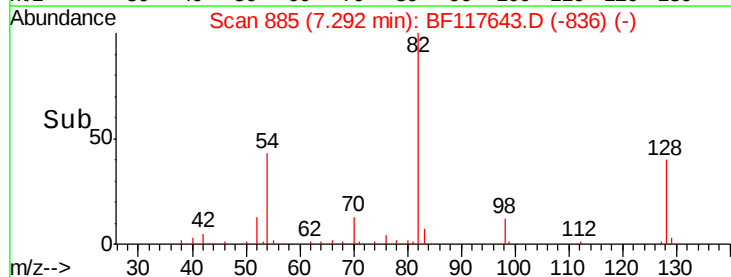


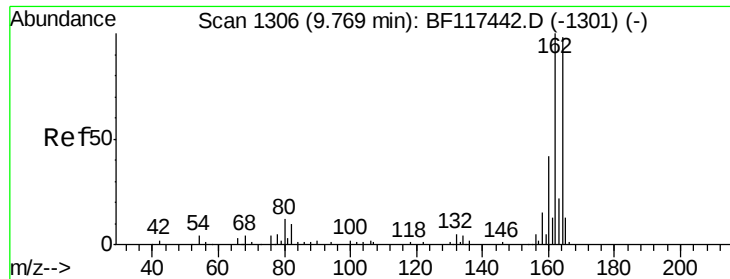




#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.76 min Scan# 1304
 Delta R.T. -0.01 min
 Lab File: BF117643.D
 Acq: 31 Oct 2019 4:01

Instrument :
 BNA_F
 ClientSampleId :
 NCQ-632

Tot Ion:164 Resp: 61649
 Ion Ratio Lower Upper
 164 100
 162 98.6 81.8 122.6
 160 41.6 34.4 51.6

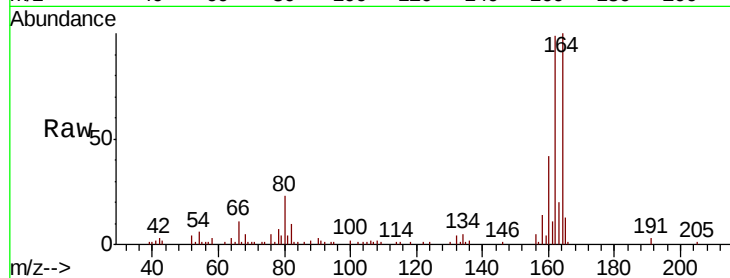


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

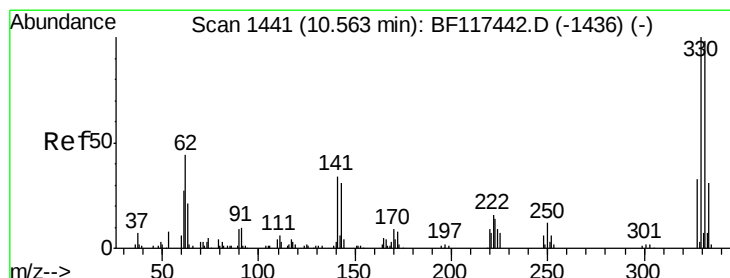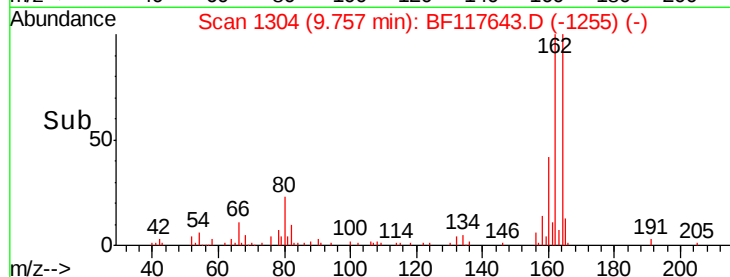
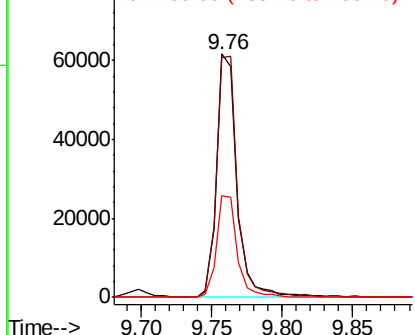


#42
 2,4,6-Tribromophenol
 Concen: 72.755 ng
 RT: 10.56 min Scan# 1440
 Delta R.T. -0.01 min
 Lab File: BF117643.D
 Acq: 31 Oct 2019 4:01

Tgt Ion:330 Resp: 38809
 Ion Ratio Lower Upper
 330 100
 332 96.8 78.5 117.7
 141 44.2 37.0 55.6

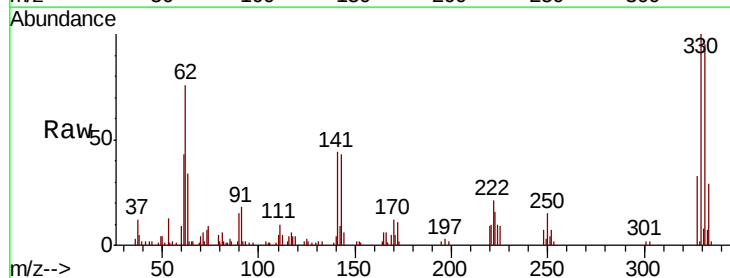

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



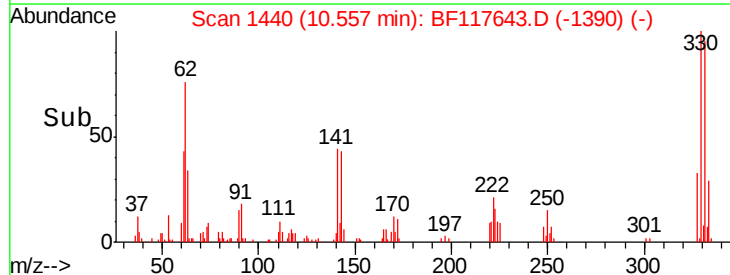
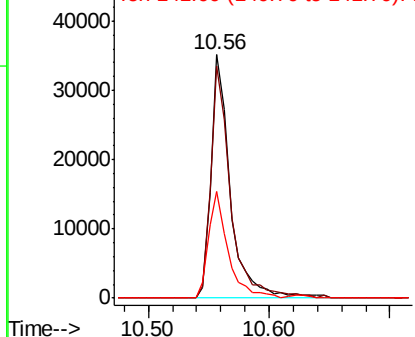




#45
2-Fluorobiphenyl
Concen: 81.576 ng
RT: 9.08 min Scan# 1189
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01




Instrument :
BNA_F
ClientSampleId :
NCQ-632


Tot Ion:172 Resp: 356927
Ion Ratio Lower Upper
172 100
171 34.8 27.5 41.3
170 22.6 18.6 27.8

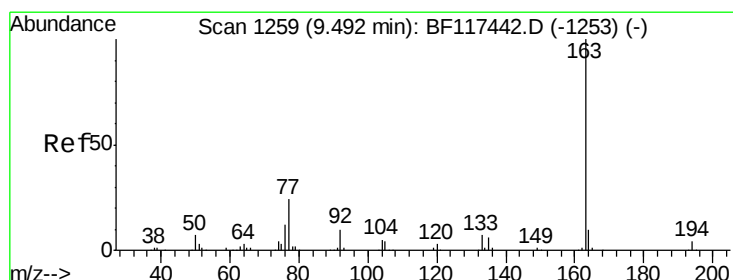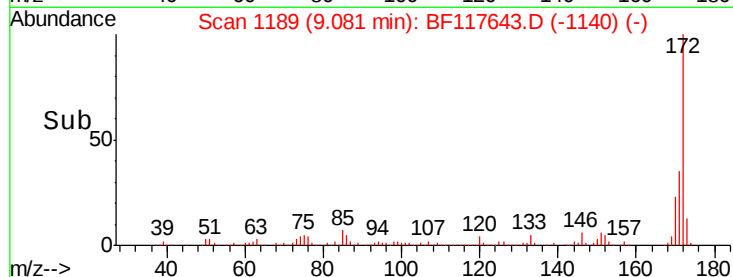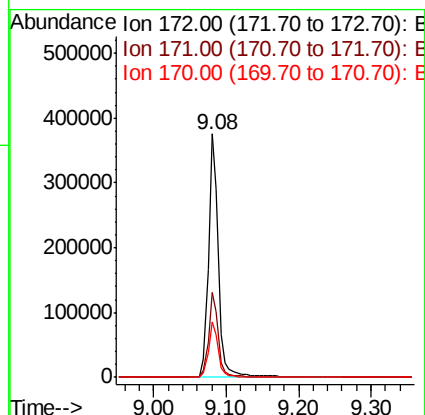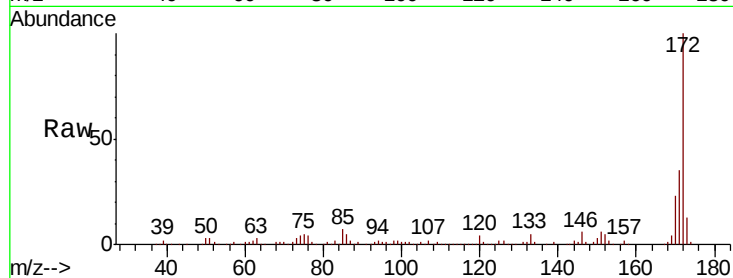

#50
Dimethylphthalate
Concen: 12.127 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Tgt Ion:163 Resp: 53298
Ion Ratio Lower Upper
163 100
194 4.4 2.9 4.3#
164 10.2 8.2 12.2

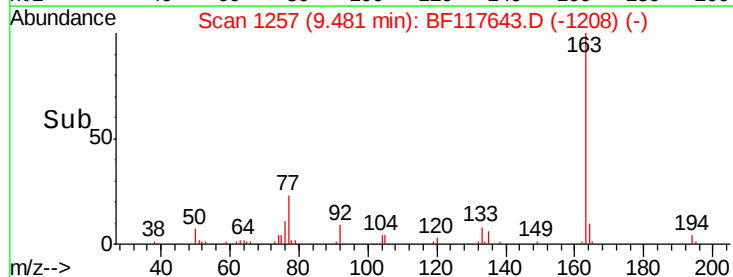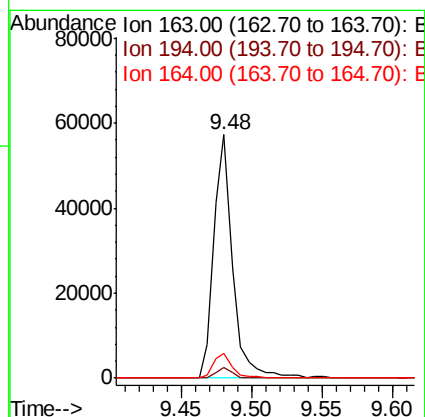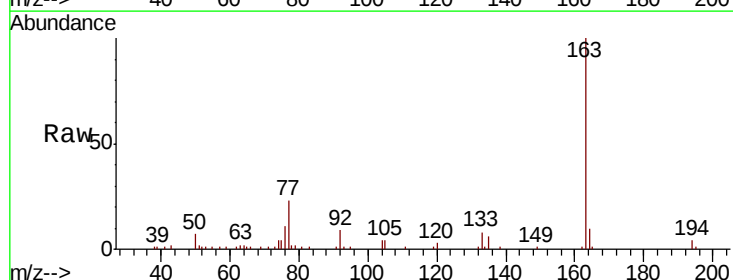


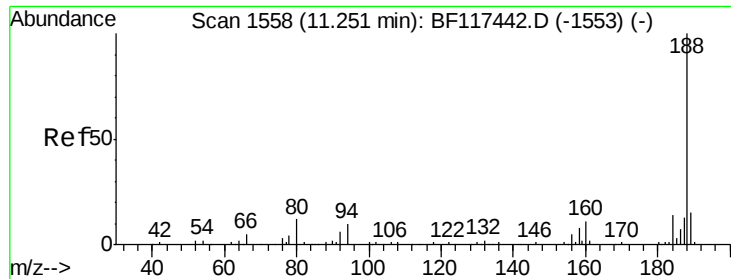




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.25 min Scan# 1558
Delta R.T. 0.00 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Instrument :
BNA_F
ClientSampleId :
NCQ-632

Tot Ion:188 Resp: 92420
Ion Ratio Lower Upper
188 100
94 9.3 8.0 12.0
80 11.0 9.5 14.3

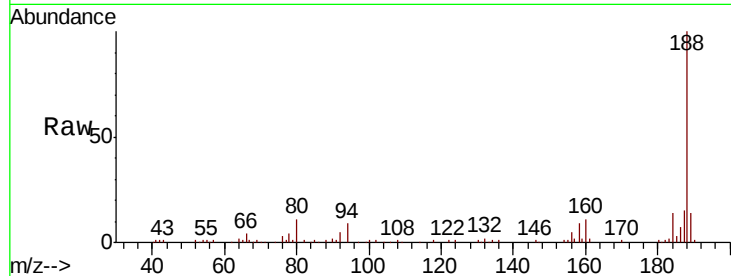


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

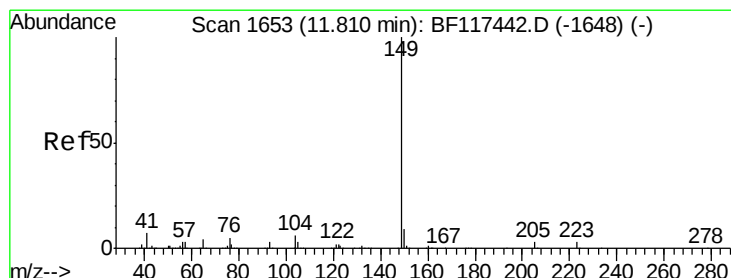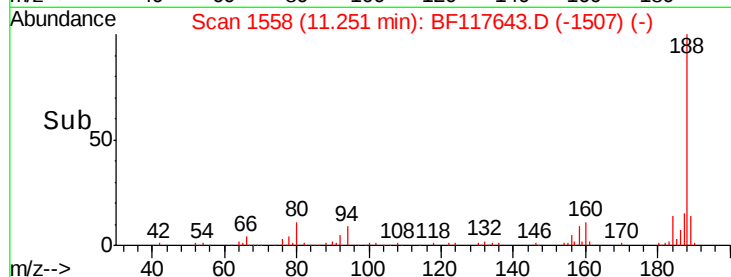
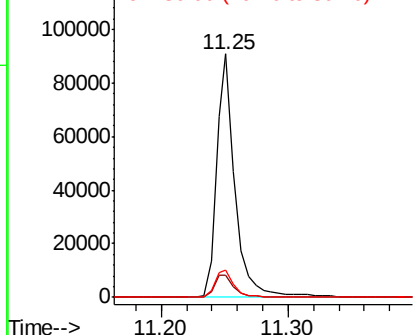



#74
Di-n-butylphthalate
Concen: 5.550 ng
RT: 11.80 min Scan# 1652
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Tgt Ion:149 Resp: 37317
Ion Ratio Lower Upper
149 100
150 9.2 7.5 11.3
104 5.1 4.6 6.8

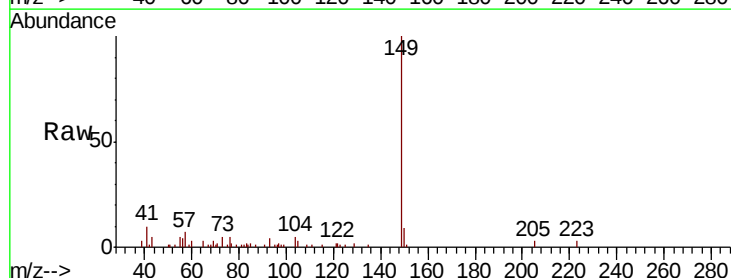

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 104.00 (103.70 to 104.70): E

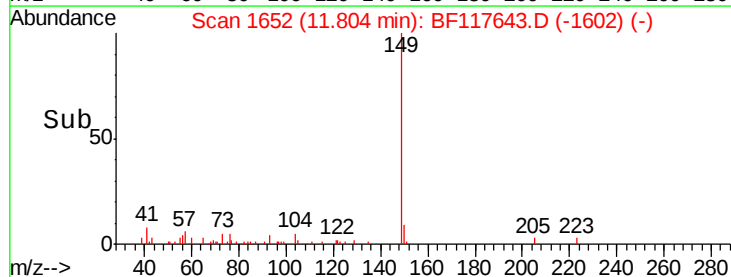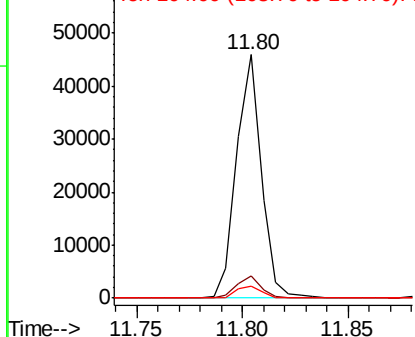


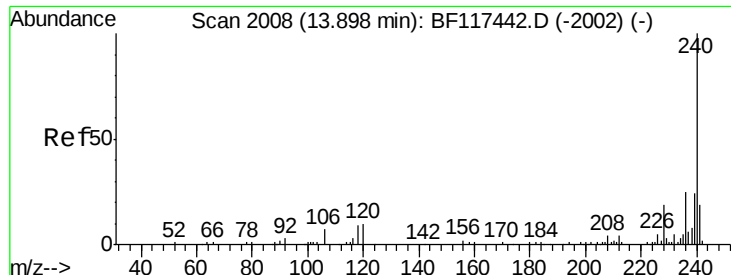




#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.90 min Scan# 2008
Delta R.T. 0.00 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Instrument :
BNA_F
ClientSampleId :
NCQ-632

Tot Ion:240 Resp: 69385
Ion Ratio Lower Upper
240 100
120 12.4 8.4 12.6
236 26.7 20.0 30.0

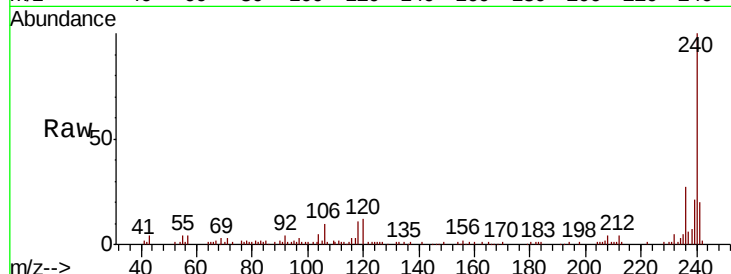


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

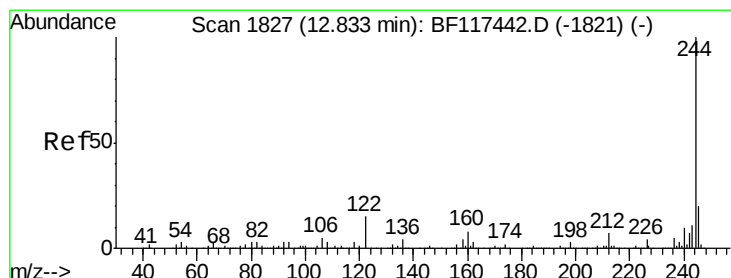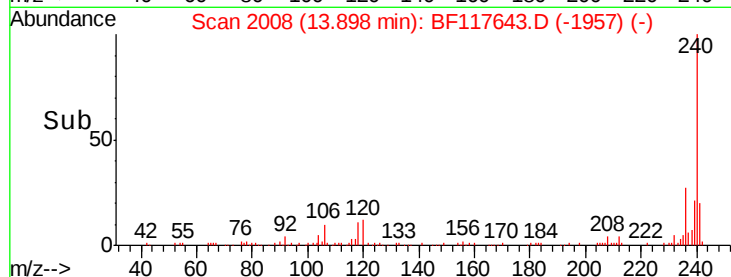
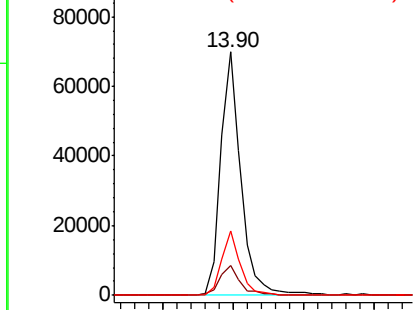



#79
Terphenyl-d14
Concen: 72.076 ng
RT: 12.83 min Scan# 1827
Delta R.T. 0.00 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Tgt Ion:244 Resp: 306599
Ion Ratio Lower Upper
244 100
212 6.9 5.8 8.6
122 12.5 11.8 17.8

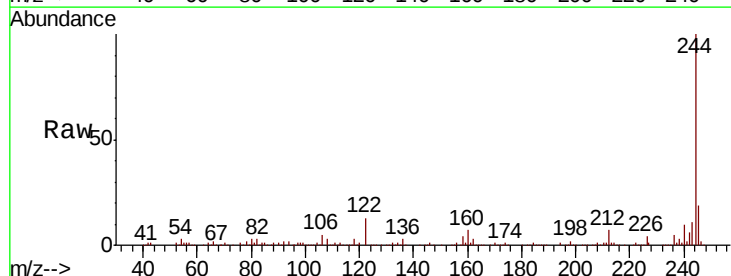

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E



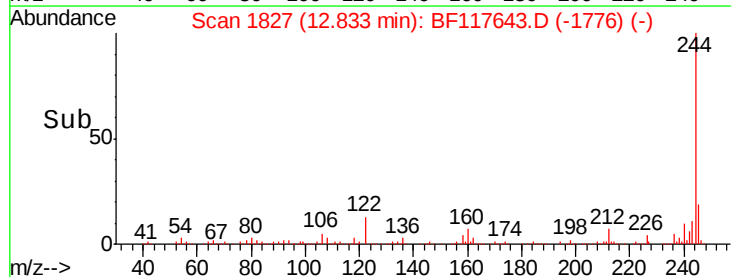
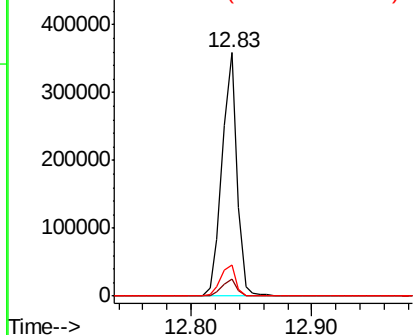


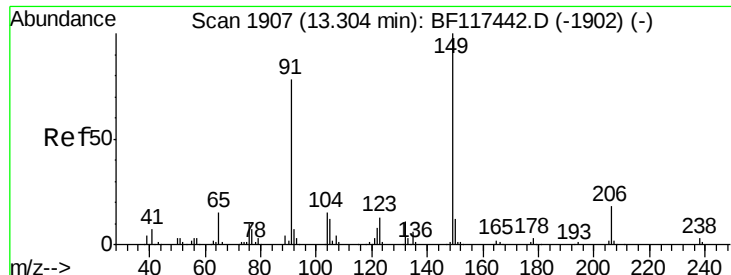

#80
Butylbenzylphthalate
Concen: 3.670 ng
RT: 13.30 min Scan# 1906
Delta R.T. -0.01 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Instrument :
BNA_F
ClientSampleId :
NCQ-632

Tot Ion:149 Resp: 10883
Ion Ratio Lower Upper
149 100
91 82.1 62.1 93.1
206 17.3 14.3 21.5

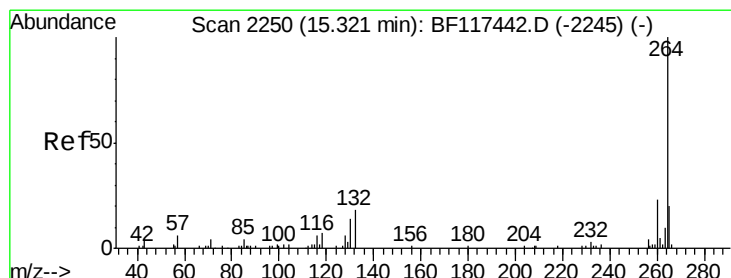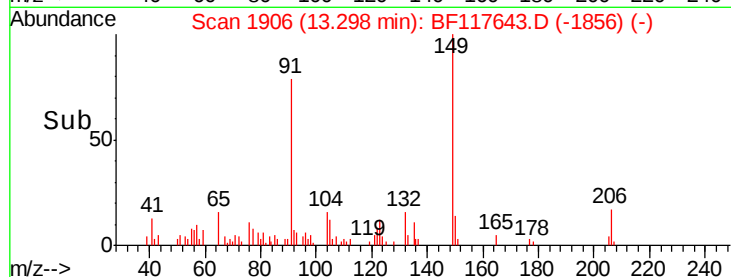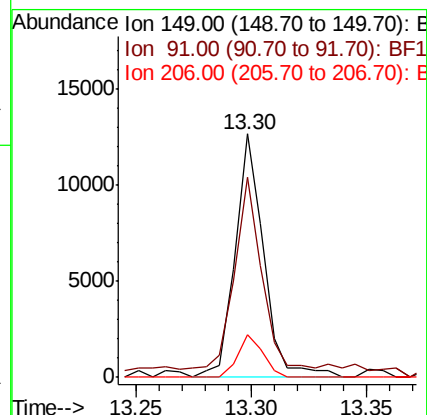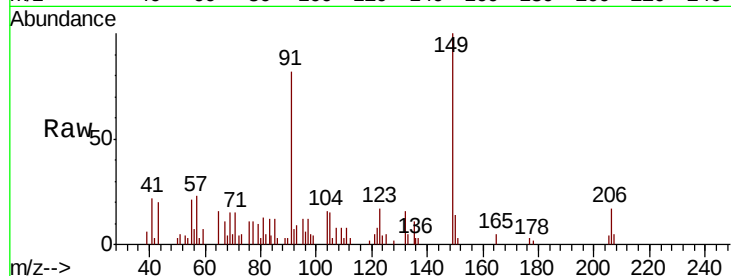

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.34 min Scan# 2253
Delta R.T. 0.02 min
Lab File: BF117643.D
Acq: 31 Oct 2019 4:01

Tgt Ion:264 Resp: 54297
Ion Ratio Lower Upper
264 100
260 27.3 18.4 27.6
265 22.3 16.1 24.1

