

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103019\
 Data File : BF117633.D
 Acq On : 30 Oct 2019 19:06
 Operator : JU
 Sample : K5140-05RE 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-102519RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	553	556	568	rBV	210839	337487	3.06%	0.733%
2	6.251	705	708	711	rBV2	110147	113165	1.03%	0.246%
3	6.316	716	719	725	rBV2	90162	113879	1.03%	0.247%
4	6.386	725	731	740	rBV2	267018	449596	4.08%	0.977%
5	6.463	740	744	748	rVV2	70410	127554	1.16%	0.277%
6	6.504	748	751	756	rVV	406506	463905	4.21%	1.008%
7	6.563	756	761	767	rVB2	523481	480846	4.36%	1.045%
8	6.739	784	791	795	rVB3	166391	261939	2.38%	0.569%
9	6.786	795	799	802	rBV	119903	113053	1.03%	0.246%
10	6.881	811	815	818	rBV2	355886	423497	3.84%	0.920%
11	7.004	832	836	839	rVB2	213536	188897	1.71%	0.410%
12	7.045	839	843	845	rVV2	125368	175883	1.60%	0.382%
13	7.069	845	847	852	rVB2	176480	164841	1.50%	0.358%
14	7.116	852	855	859	rBV2	340327	322330	2.92%	0.700%
15	7.263	875	880	883	rBV	205844	250422	2.27%	0.544%
16	7.292	883	885	888	rVV2	224005	285854	2.59%	0.621%
17	7.328	888	891	894	rVV	824197	653533	5.93%	1.420%
18	7.375	894	899	902	rVB4	159800	223681	2.03%	0.486%
19	7.416	902	906	908	rBV4	90212	129553	1.18%	0.281%
20	7.510	919	922	923	rVV2	93871	114422	1.04%	0.249%
21	7.528	923	925	929	rVB	293115	269670	2.45%	0.586%
22	7.628	936	942	944	rBV3	142724	258147	2.34%	0.561%
23	7.692	950	953	956	rVB3	185763	205664	1.87%	0.447%
24	7.728	956	959	961	rBV2	216746	198173	1.80%	0.430%
25	7.763	961	965	969	rVV5	241261	412284	3.74%	0.896%
26	7.804	969	972	974	rVV2	138575	131203	1.19%	0.285%
27	7.963	993	999	1001	rBV5	128919	201103	1.82%	0.437%
28	7.998	1001	1005	1009	rVV2	810708	916430	8.32%	1.991%
29	8.057	1013	1015	1016	rVV	181673	153788	1.40%	0.334%
30	8.075	1016	1018	1020	rVB	285186	212438	1.93%	0.461%
31	8.098	1020	1022	1025	rBV3	129086	126996	1.15%	0.276%
32	8.181	1031	1036	1038	rBV4	77444	117147	1.06%	0.254%
33	8.210	1038	1041	1044	rVV3	176696	180254	1.64%	0.392%
34	8.298	1052	1056	1063	rVV5	243518	467742	4.24%	1.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103019\
 Data File : BF117633.D
 Acq On : 30 Oct 2019 19:06
 Operator : JU
 Sample : K5140-05RE 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-102519RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.357	1063	1066	1069	rVV3	221611	213290	1.94%	0.463%
36	8.392	1069	1072	1075	rVV3	245704	267283	2.43%	0.581%
37	8.433	1075	1079	1081	rVV2	322431	345808	3.14%	0.751%
38	8.516	1089	1093	1095	rBV2	287856	271360	2.46%	0.589%
39	8.604	1104	1108	1111	rBV	791675	684787	6.21%	1.488%
40	8.833	1144	1147	1151	rBV3	199087	171967	1.56%	0.374%
41	8.963	1165	1169	1173	rVB4	155808	218810	1.99%	0.475%
42	9.028	1178	1180	1187	rVB3	237074	259125	2.35%	0.563%
43	9.080	1187	1189	1194	rBV	387900	345490	3.14%	0.750%
44	9.169	1199	1204	1208	rBV	568648	606127	5.50%	1.317%
45	9.233	1213	1215	1218	rVB2	142506	121658	1.10%	0.264%
46	9.480	1253	1257	1259	rBV3	231535	283066	2.57%	0.615%
47	9.504	1259	1261	1265	rVV2	129741	143087	1.30%	0.311%
48	9.539	1265	1267	1270	rVB	138295	113097	1.03%	0.246%
49	9.692	1290	1293	1296	rBV	461734	339568	3.08%	0.738%
50	9.763	1302	1305	1309	rVB	162380	148014	1.34%	0.322%
51	10.016	1344	1348	1351	rBV4	104725	132926	1.21%	0.289%
52	10.192	1375	1378	1381	rVB	367396	269393	2.44%	0.585%
53	10.410	1410	1415	1420	rVB	114860	158740	1.44%	0.345%
54	10.557	1437	1440	1446	rBV2	155362	208099	1.89%	0.452%
55	10.663	1455	1458	1467	rVB	321576	376962	3.42%	0.819%
56	11.110	1531	1534	1537	rBV	270677	219400	1.99%	0.477%
57	11.139	1537	1539	1545	rVB2	108772	123051	1.12%	0.267%
58	11.251	1555	1558	1560	rBV	152874	135768	1.23%	0.295%
59	11.274	1560	1562	1569	rVB	126590	146059	1.33%	0.317%
60	11.533	1603	1606	1608	rBV	215128	177858	1.61%	0.386%
61	11.557	1608	1610	1613	rVB	150814	119755	1.09%	0.260%
62	11.645	1620	1625	1628	rBV	3576253	3391913	30.78%	7.368%
63	11.786	1646	1649	1654	rVB	121152	122786	1.11%	0.267%
64	11.939	1672	1675	1681	rVB	172845	189591	1.72%	0.412%
65	12.351	1736	1745	1746	rBV2	5549796	11020341	100.00%	23.939%
66	12.380	1746	1750	1753	rVV	7530671	10391444	94.29%	22.573%
67	12.433	1756	1759	1763	rVB	1572870	1422785	12.91%	3.091%
68	12.474	1763	1766	1768	rBV2	261161	324937	2.95%	0.706%
69	12.498	1768	1770	1780	rVB	345999	423167	3.84%	0.919%
70	12.663	1795	1798	1801	rBV	131907	126476	1.15%	0.275%
71	12.704	1802	1805	1812	rVB	244755	286719	2.60%	0.623%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103019\
Data File : BF117633.D
Acq On : 30 Oct 2019 19:06
Operator : JU
Sample : K5140-05RE 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-102519RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.833	1824	1827	1830	rVB	367709	306949	2.79%	0.667%
73	13.015	1855	1858	1859	rVV2	101065	120134	1.09%	0.261%
74	13.074	1863	1868	1871	rBV2	255040	327882	2.98%	0.712%
75	13.151	1878	1881	1885	rVB	220010	188207	1.71%	0.409%
76	13.821	1991	1995	2002	rBV	200128	227570	2.06%	0.494%
77	13.898	2004	2008	2011	rBV3	131728	186290	1.69%	0.405%
78	14.351	2081	2085	2088	rBV	175775	217025	1.97%	0.471%
79	14.645	2132	2135	2138	rBV	136869	122158	1.11%	0.265%
80	14.757	2150	2154	2161	rVB	208663	271925	2.47%	0.591%
81	14.962	2186	2189	2195	rVB2	137963	166799	1.51%	0.362%
82	15.315	2246	2249	2252	rBV	97592	114039	1.03%	0.248%
83	16.362	2424	2427	2436	rVB3	65731	117073	1.06%	0.254%
84	16.739	2488	2491	2501	rVB9	48750	123425	1.12%	0.268%


Sum of corrected areas: 46035559

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103019\
Data File : BF117633.D
Acq On : 30 Oct 2019 19:06
Operator : JU
Sample : K5140-05RE 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-102519RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

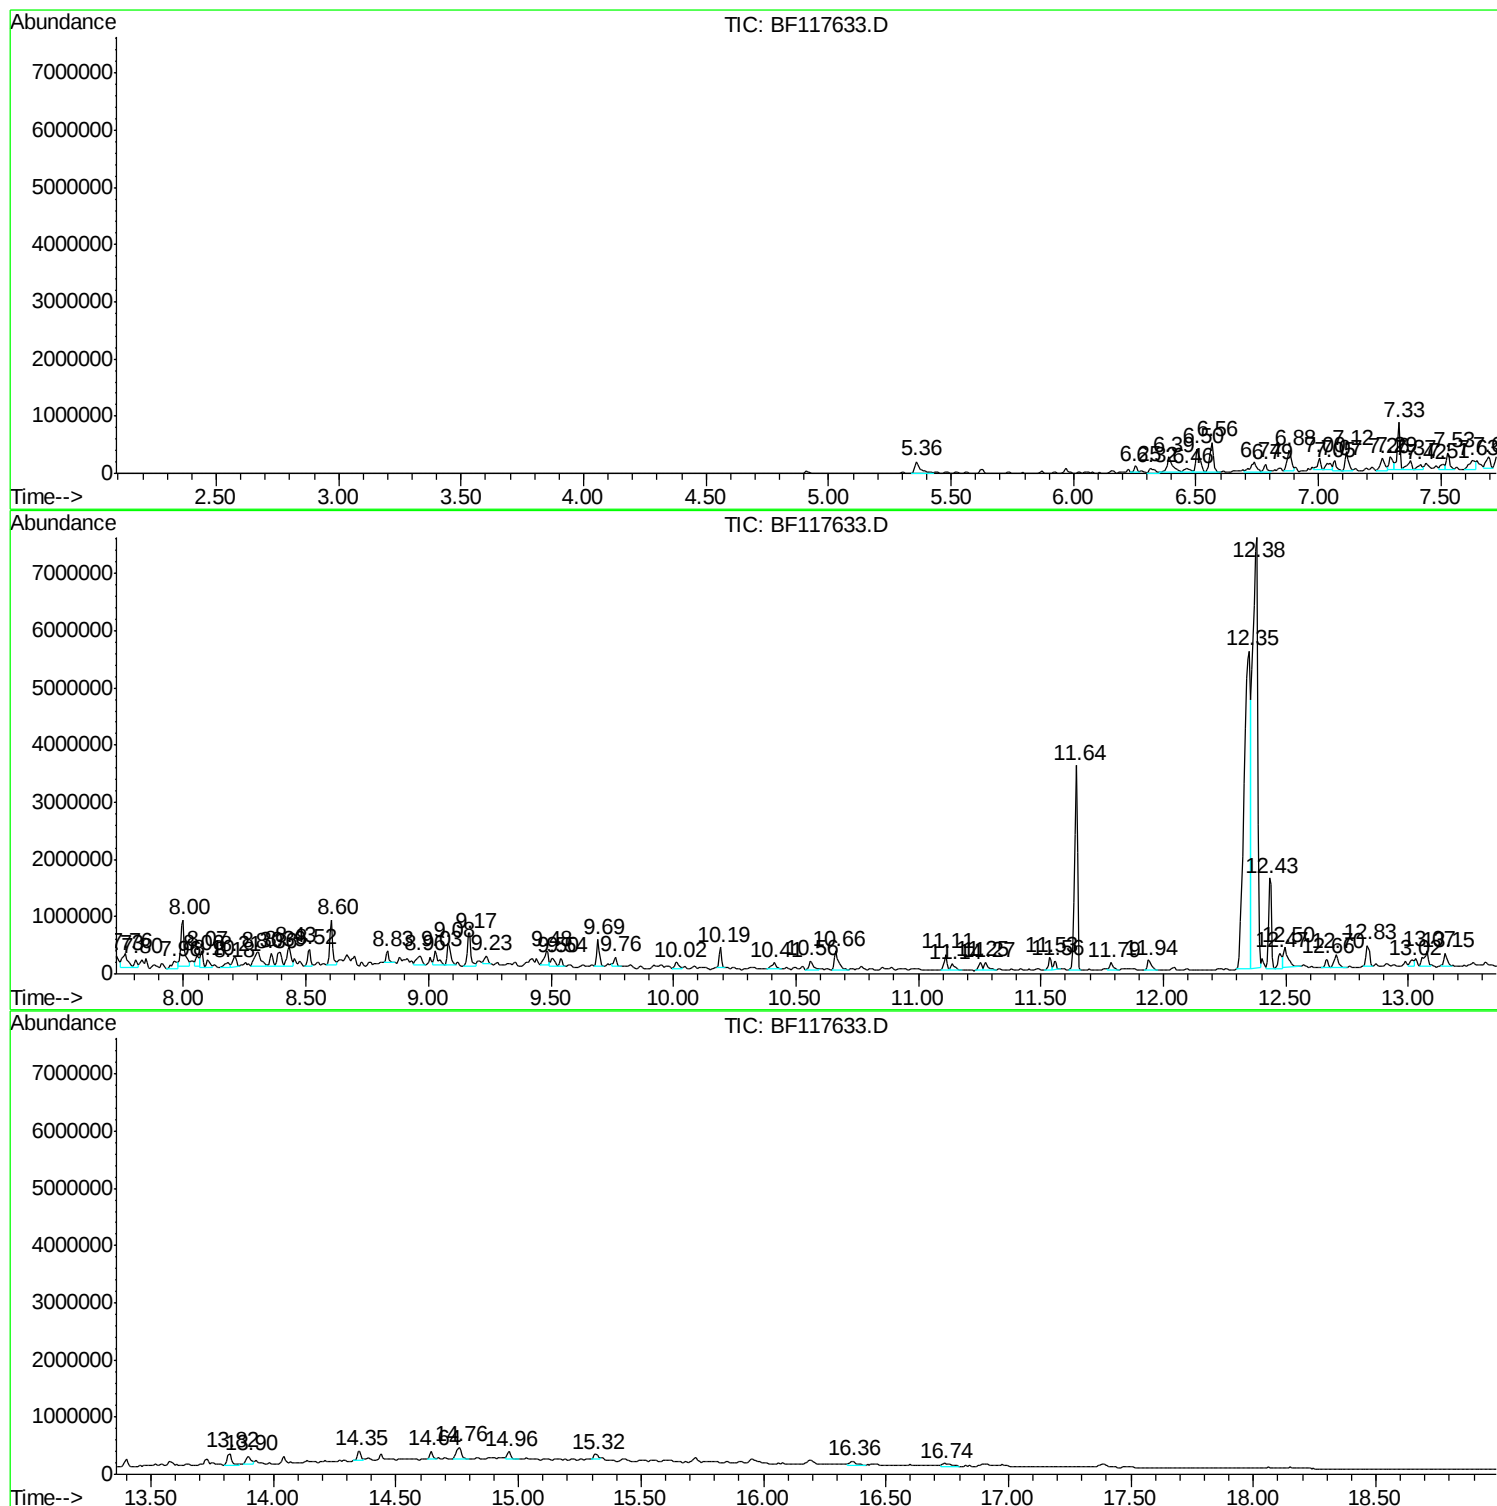

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103019\
Data_File : BF117633.D
Acq_On : 30-Oct-2019 19:066
Operator : JUJ
Sample : K5140-05RE_2XX
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
HR-06-102519RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
