


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103019\
 Data File : BF117637.D
 Acq On : 30 Oct 2019 21:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

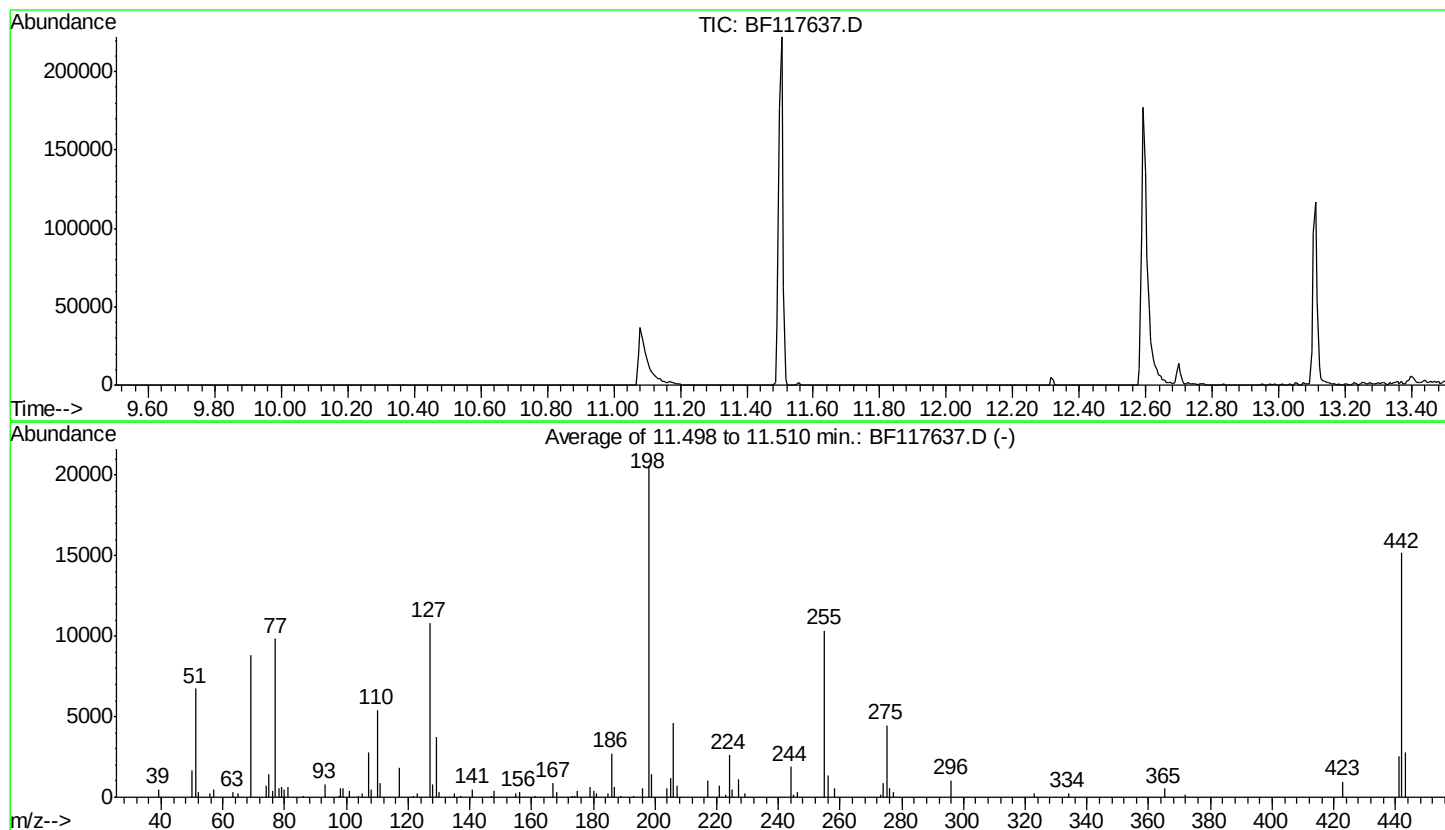

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	6733	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.8	8800	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	10840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20580	PASS
199	198	5	9	6.8	1394	PASS
275	198	10	60	21.8	4487	PASS
365	198	1	100	2.6	531	PASS
441	198	0.01	100	12.3	2537	PASS
442	198	50	100	73.6	15138	PASS
443	442	15	24	18.4	2782	PASS