
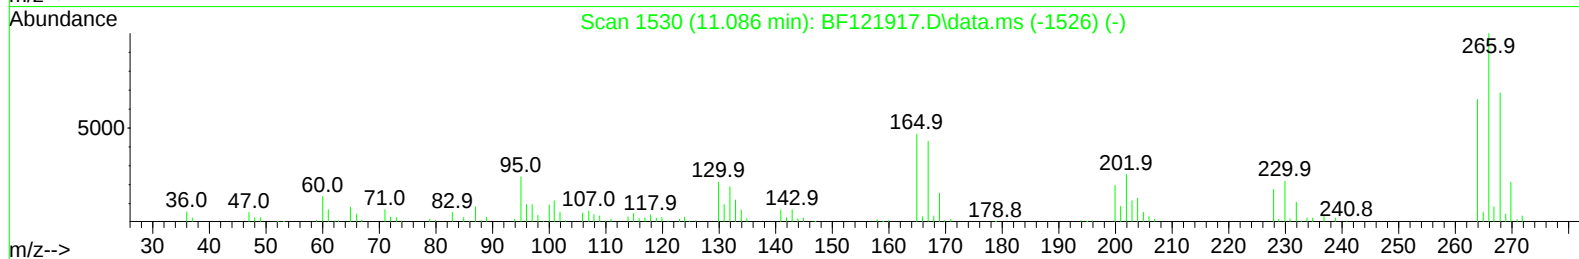
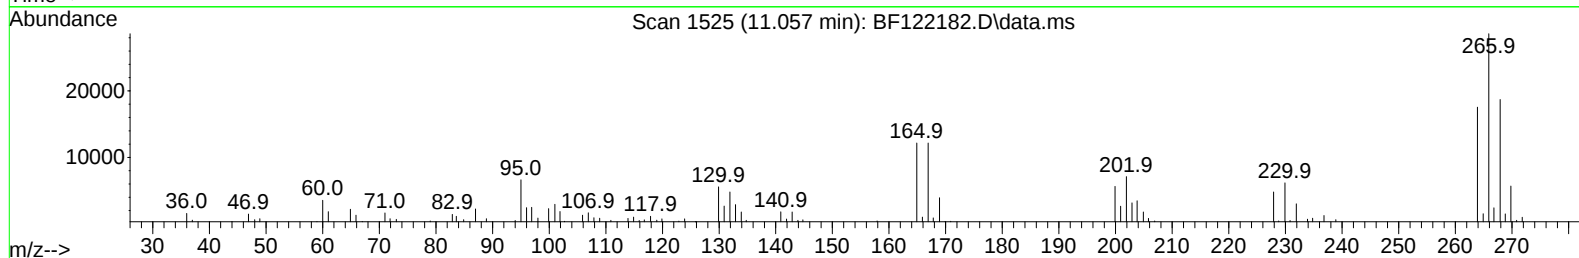


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122182.D
Acq On : 30 Oct 2020 15:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 03:30:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

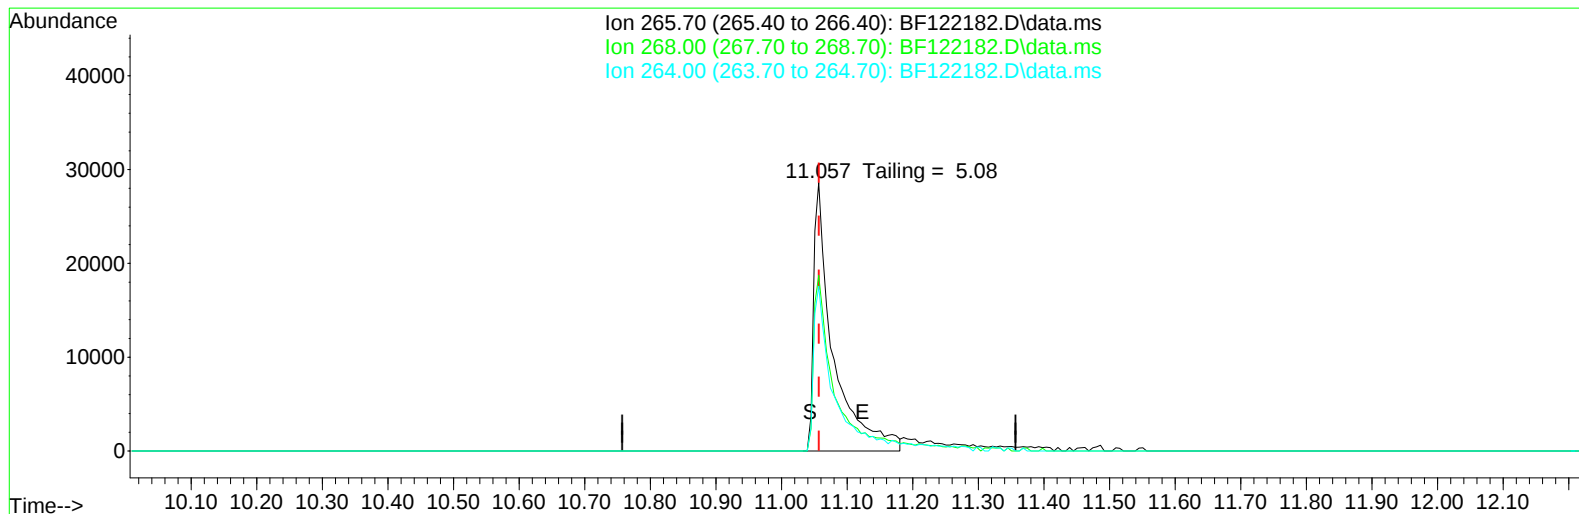

TIC: BF122182.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.000) 88935.35 ng

response 61424

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	65.38
264.00	62.40	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122182.D
Acq On : 30 Oct 2020 15:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 03:30:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

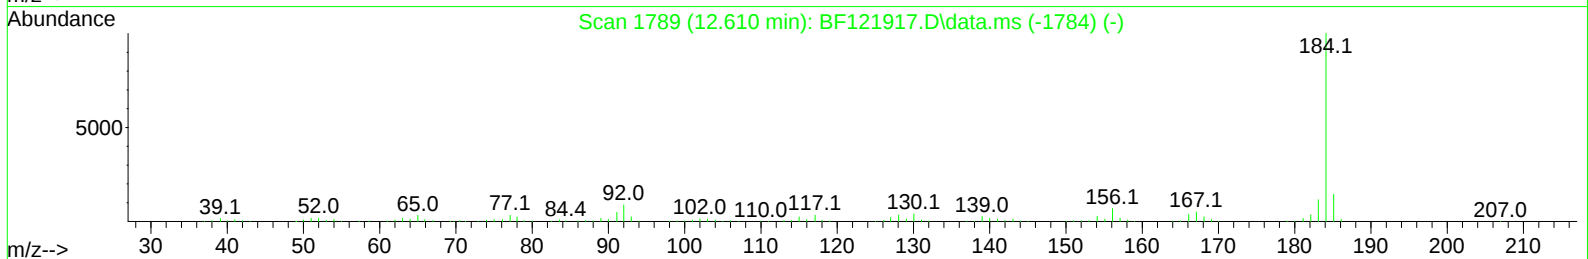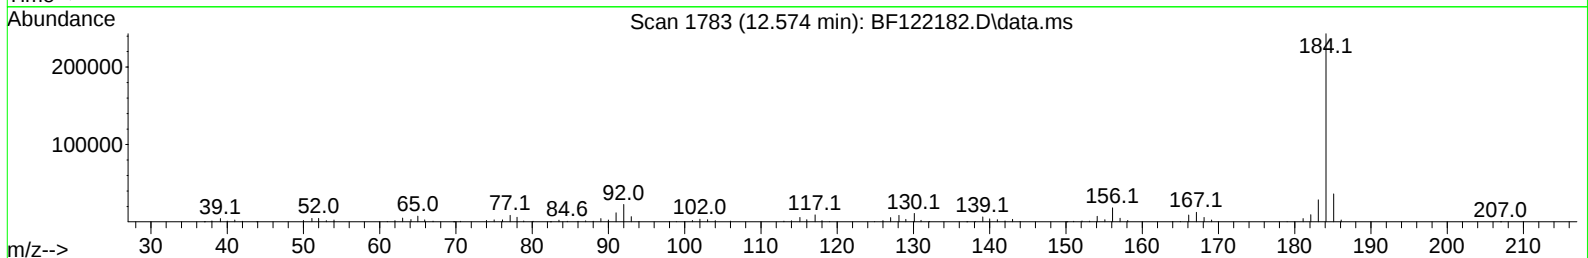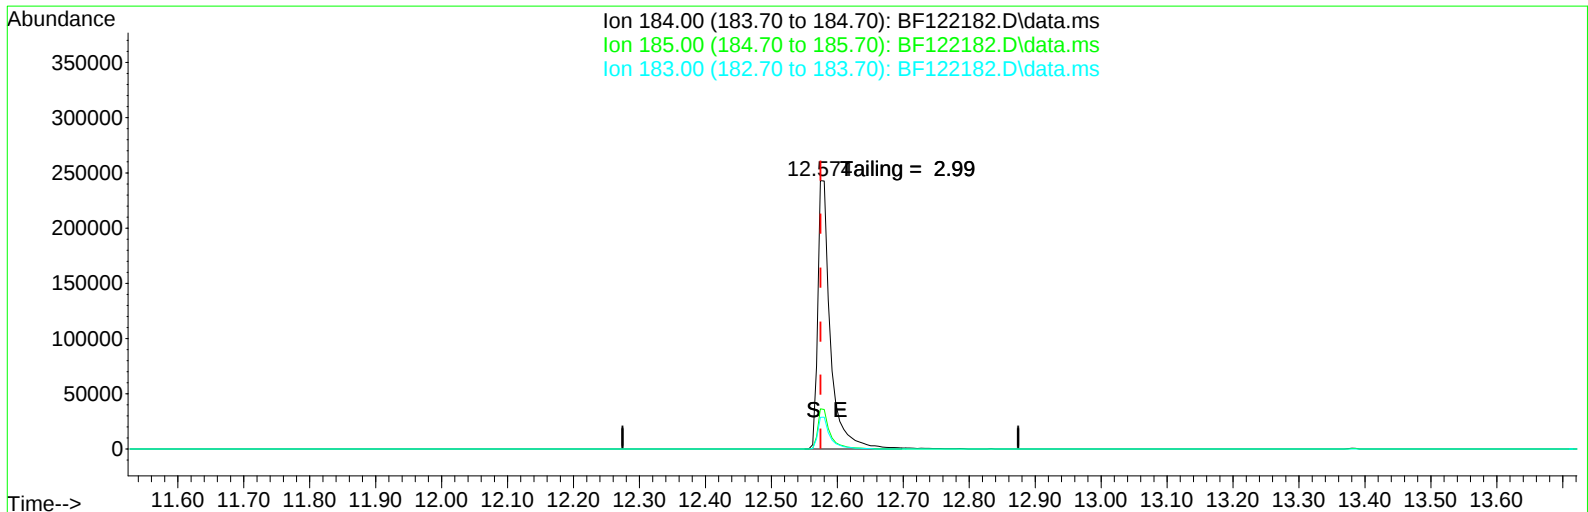

TIC: BF122182.D\data.ms

(77) Benzidine

12.574min (-0.000) 0.00 ng

response 324738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.96
183.00	11.70	11.81
0.00	0.00	0.00