

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122185.D
 Acq On : 30 Oct 2020 17:42
 Operator : JU/CG
 Sample : L4532-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 IB1-TREATED-EFFLU

Manual Integrations
 APPROVED

mohammad
 11/2/2020 12:36:05 PM

Quant Time: Oct 30 18:09:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 30 10:16:54 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.710	152	104215	20.00	ng	0.00
21) Naphthalene-d8	7.992	136	416856	20.00	ng	0.00
39) Acenaphthene-d10	9.745	164	215048	20.00	ng	0.00
64) Phenanthrene-d10	11.233	188	400376	20.00	ng	0.00
76) Chrysene-d12	13.880	240	292620	20.00	ng	0.00
86) Perylene-d12	15.321	264	243465	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.339	112	482176	68.29	ng	0.00
7) Phenol-d6	6.369	99	396696	43.64	ng	0.00
23) Nitrobenzene-d5	7.281	82	728406	89.61	ng	0.00
42) 2,4,6-Tribromophenol	10.545	330	349193	131.27	ng	0.00
45) 2-Fluorobiphenyl	9.069	172	1205125	82.45	ng	0.00
79) Terphenyl-d14	12.821	244	1203295	78.37	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	9.469	163	140829	8.96	ng	99
87) Indeno(1,2,3-cd)pyrene	16.745	276	123247	7.80	ng	98
88) Benzo(b)fluoranthene	14.921	252	36871	2.24	ng	99
89) Benzo(k)fluoranthene	14.945	252	38433m	2.46	ng	
90) Benzo(a)pyrene	15.268	252	40195	2.83	ng	97
91) Dibenzo(a,h)anthracene	16.745	278	91859	7.06	ng	98
92) Benzo(g,h,i)perylene	17.174	276	121903	9.36	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122185.D
Acq On : 30 Oct 2020 17:42
Operator : JU/CG
Sample : L4532-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU

Manual Integrations
APPROVED

mohammad
11/2/2020 12:36:05 PM

Quant Time: Oct 30 18:09:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

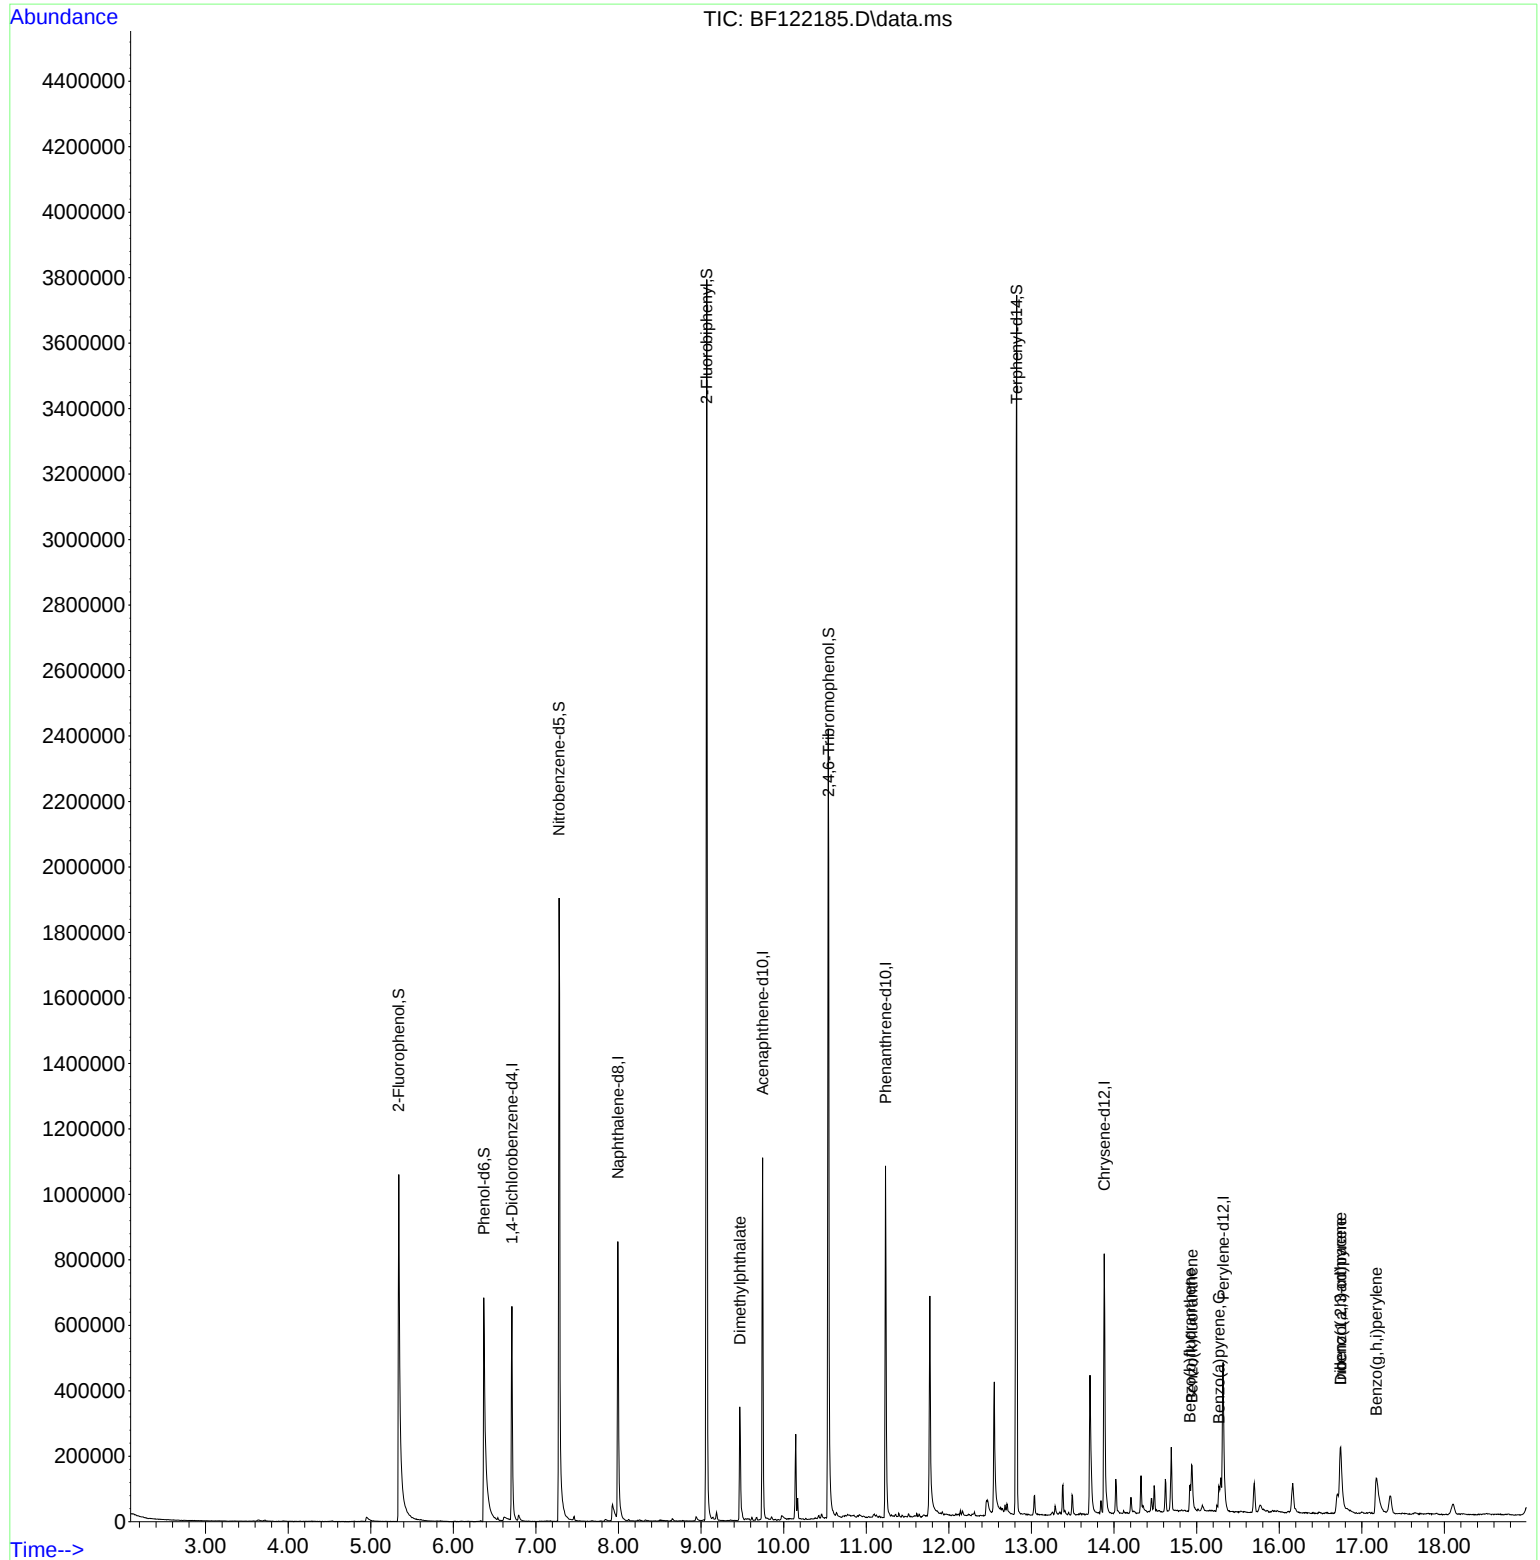







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.710 min Scan# 786
Delta R.T. -0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:152 Resp: 104215
Ion Ratio Lower Upper
152 100
150 158.3 125.3 187.9
115 62.1 51.9 77.9

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:05 PM

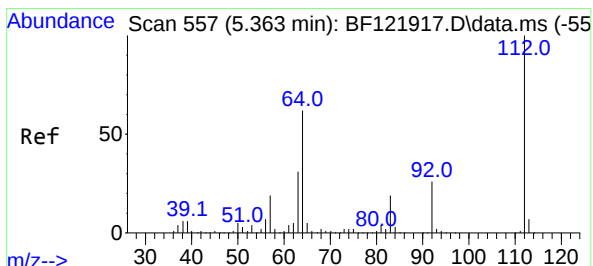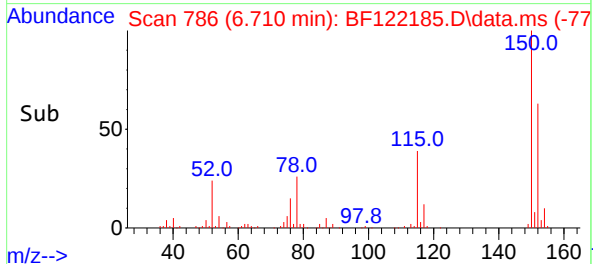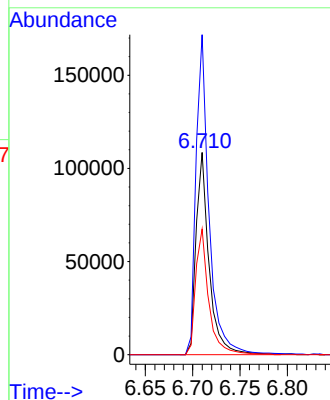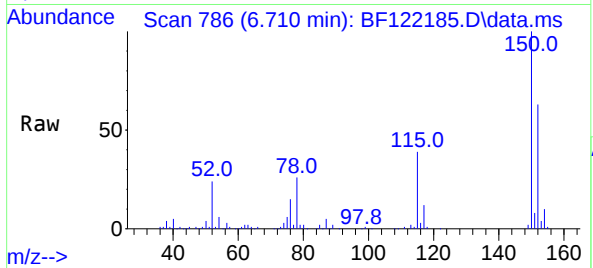

#5
2-Fluorophenol
Concen: 68.29 ng
RT: 5.339 min Scan# 553
Delta R.T. 0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:112 Resp: 482176
Ion Ratio Lower Upper
112 100
64 63.0 50.4 75.6
63 32.4 25.8 38.6

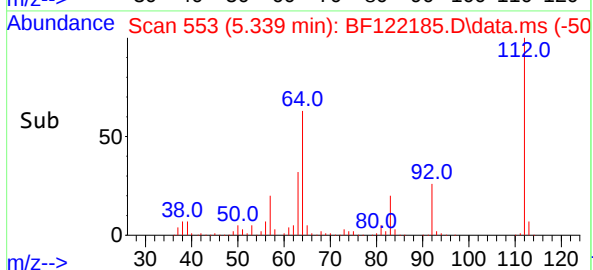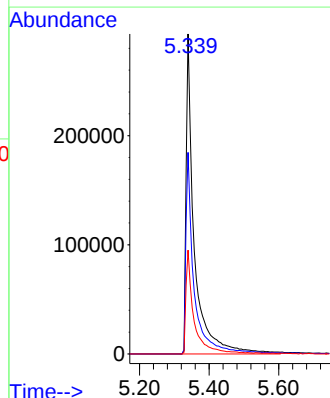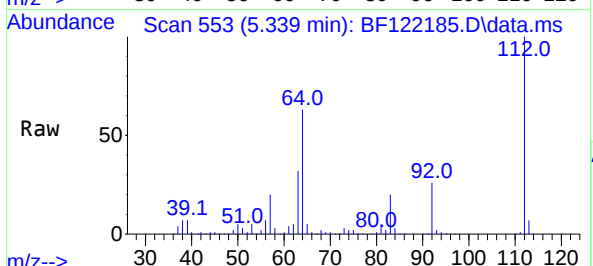







#7
Phenol-d6
Concen: 43.64 ng
RT: 6.369 min Scan# 728
Delta R.T. -0.000 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion: 99 Resp: 396696
Ion Ratio Lower Upper
99 100
42 20.9 15.9 23.9
71 35.0 27.1 40.7

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:05 PM

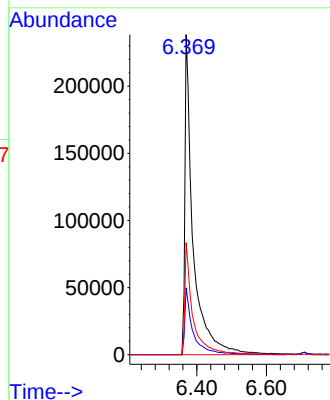

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.992 min Scan# 1004
Delta R.T. -0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion: 136 Resp: 416856
Ion Ratio Lower Upper
136 100
137 11.2 8.6 13.0
54 9.7 7.1 10.7
68 6.4 5.0 7.4

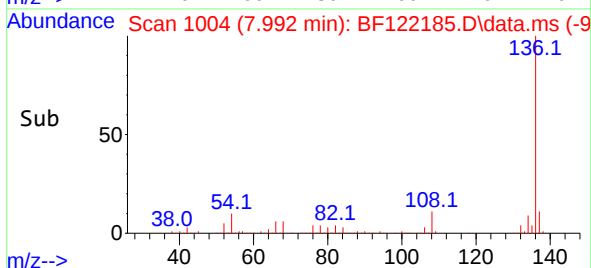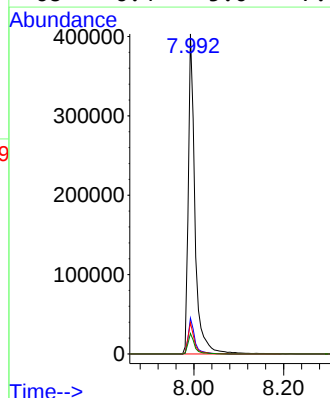

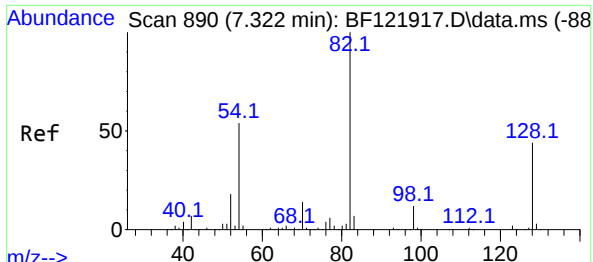

#23
Nitrobenzene-d5
Concen: 89.61 ng
RT: 7.281 min Scan# 883
Delta R.T. -0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42





Tgt Ion: 82 Resp: 728406

Ion	Ratio	Lower	Upper
82	100		
128	41.1	35.0	52.4
54	55.3	43.9	65.9

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU

Manual Integrations
APPROVED




mohammad
11/2/2020 12:36:05 PM

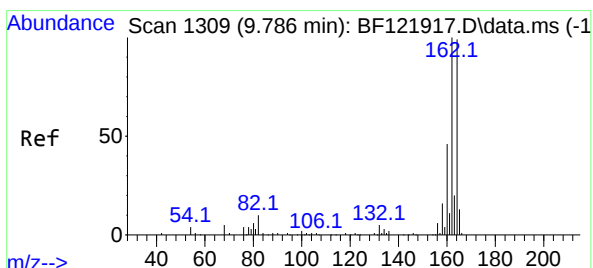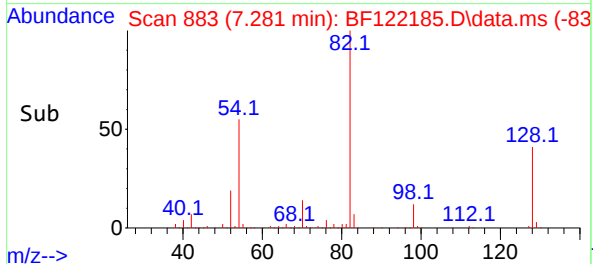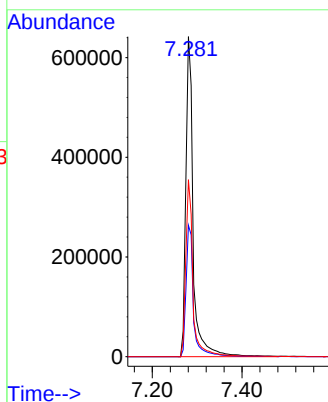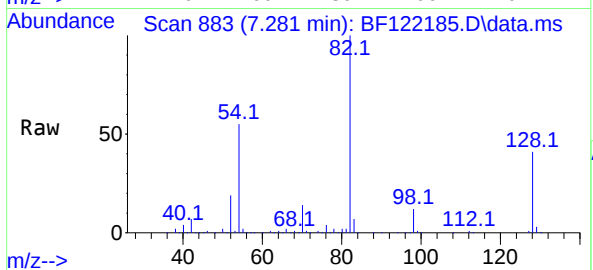


#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.745 min Scan# 1302
Delta R.T. -0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion: 164 Resp: 215048


Ion	Ratio	Lower	Upper
164	100		
162	103.1	83.2	124.8
160	46.8	37.5	56.3

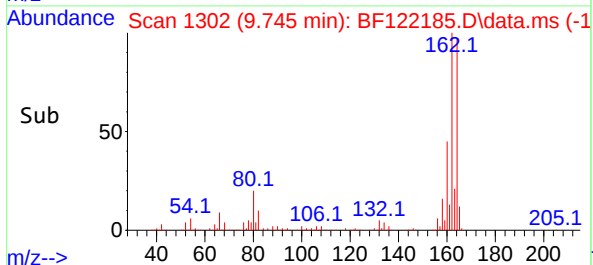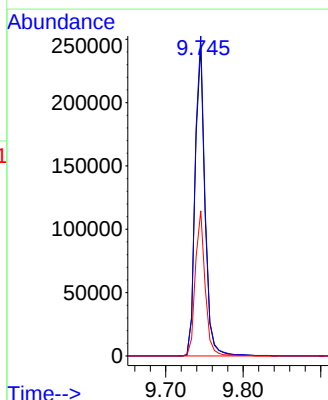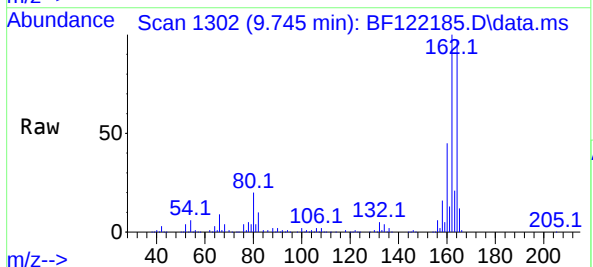



#42
2,4,6-Tribromophenol
Concen: 131.27 ng
RT: 10.545 min Scan# 1438
Delta R.T. -0.000 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42




Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU

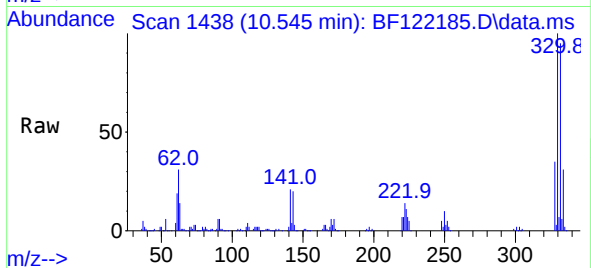


Tgt Ion: 330 Resp: 349193
Ion Ratio Lower Upper
330 100
332 95.2 77.3 115.9
141 29.0 22.3 33.5

Manual Integrations
APPROVED



mohammad
11/2/2020 12:36:05 PM

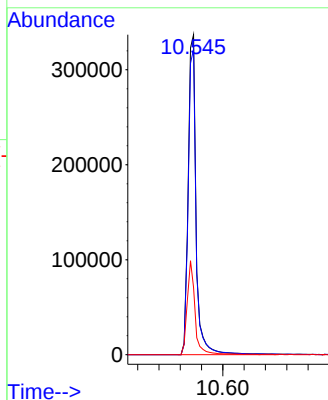

#45
2-Fluorobiphenyl
Concen: 82.45 ng
RT: 9.069 min Scan# 1187
Delta R.T. -0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42



Tgt Ion: 172 Resp: 1205125
Ion Ratio Lower Upper
172 100
171 36.2 29.1 43.7
170 24.1 19.8 29.6

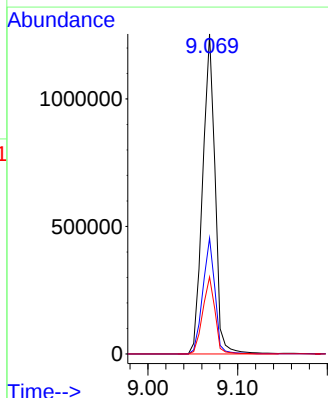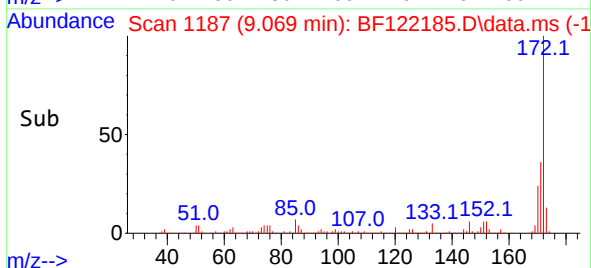







#50
Dimethylphthalate
Concen: 8.96 ng
RT: 9.469 min Scan# 1255
Delta R.T. -0.012 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:163 Resp: 140829
Ion Ratio Lower Upper
163 100
194 3.7 3.3 4.9
164 10.4 8.2 12.4

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:05 PM

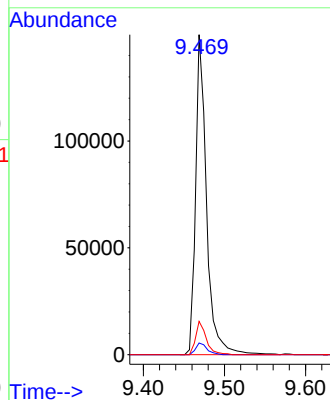

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.233 min Scan# 1555
Delta R.T. -0.000 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:188 Resp: 400376
Ion Ratio Lower Upper
188 100
94 10.0 8.3 12.5
80 10.9 9.1 13.7

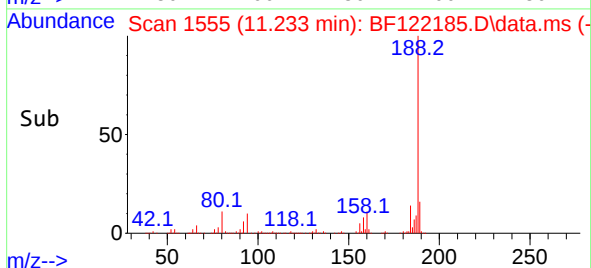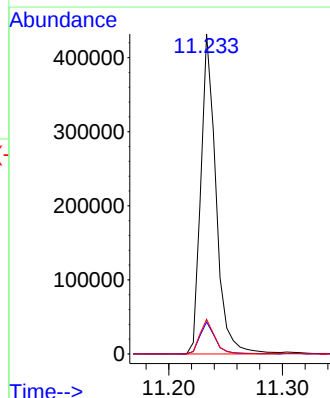







#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.880 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:240 Resp: 292620
Ion Ratio Lower Upper
240 100
120 11.2 9.2 13.8
236 25.7 20.9 31.3

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:05 PM

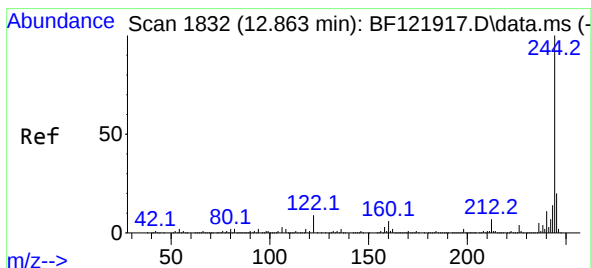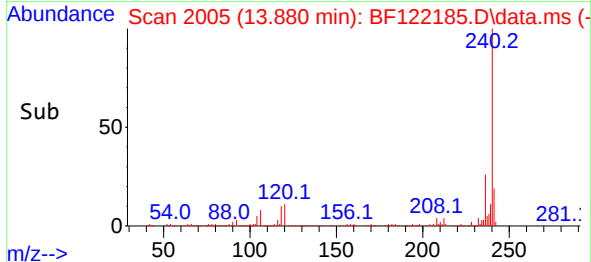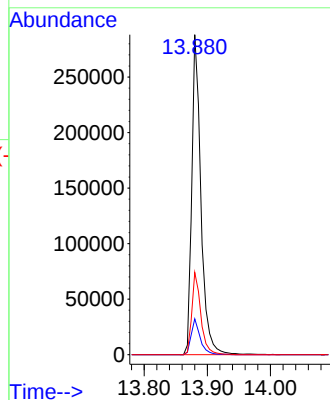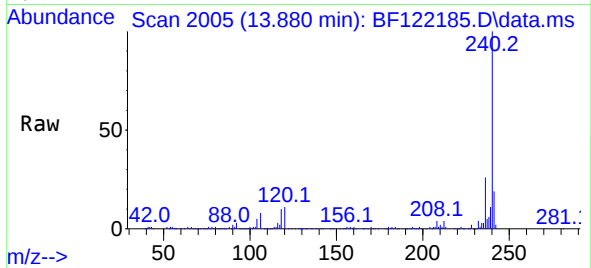


#79
Terphenyl-d14
Concen: 78.37 ng
RT: 12.821 min Scan# 1825
Delta R.T. 0.006 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:244 Resp: 1203295
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.2
122 9.3 8.1 12.1

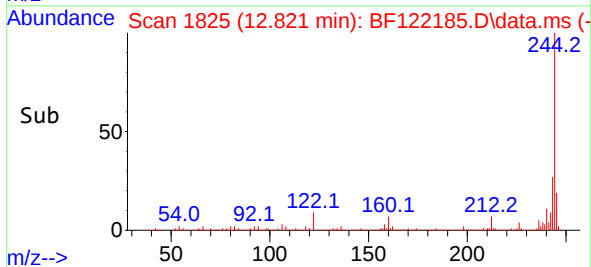
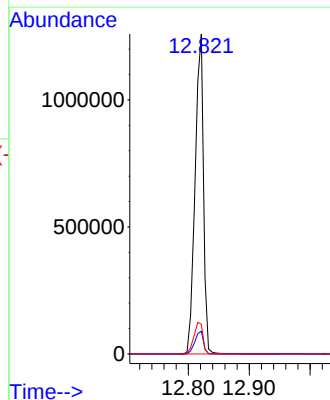
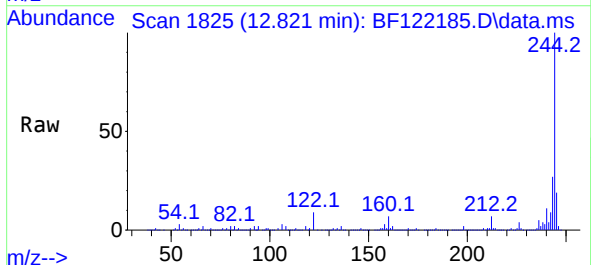





#86
Perylene-d12
Concen: 20.00 ng
RT: 15.321 min Scan# 2250
Delta R.T. 0.017 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

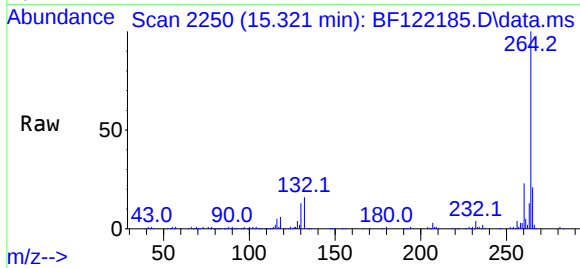



Tgt Ion:264 Resp: 243465
Ion Ratio Lower Upper
264 100
260 23.5 18.7 28.1
265 21.1 17.3 25.9

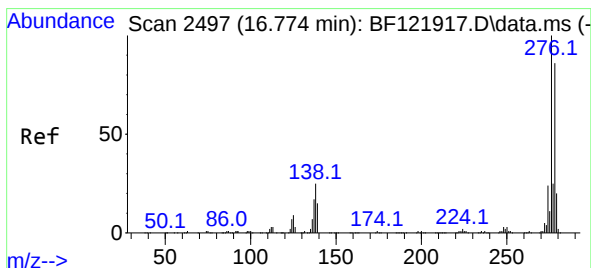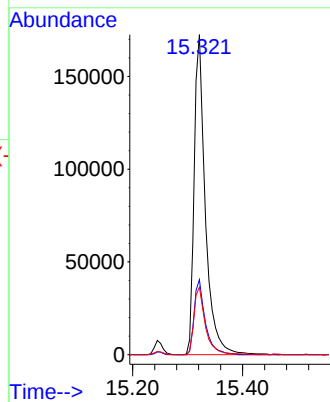

#87
Indeno(1,2,3-cd)pyrene
Concen: 7.80 ng
RT: 16.745 min Scan# 2492
Delta R.T. 0.029 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

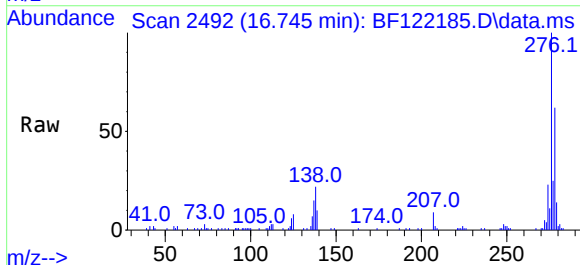


Tgt Ion:276 Resp: 123247
Ion Ratio Lower Upper
276 100
138 23.4 19.9 29.9
277 24.7 20.4 30.6

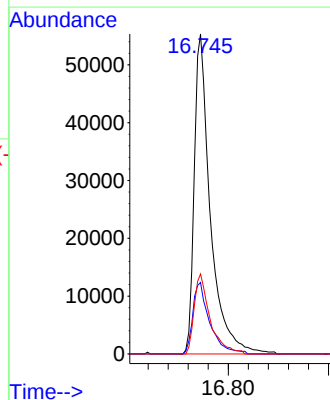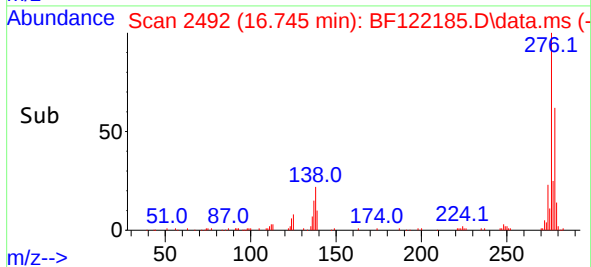

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU

Manual Integrations
APPROVED

mohammad
11/2/2020 12:36:05 PM







#88
Benzo(b)fluoranthene
Concen: 2.24 ng
RT: 14.921 min Scan# 2182
Delta R.T. 0.023 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:252 Resp: 36871
Ion Ratio Lower Upper
252 100
253 22.9 18.2 27.2
125 11.1 8.0 12.0

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:05 PM

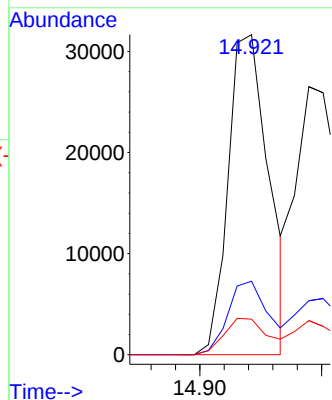

#89
Benzo(k)fluoranthene
Concen: 2.46 ng m
RT: 14.945 min Scan# 2186
Delta R.T. 0.017 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:252 Resp: 38433
Ion Ratio Lower Upper
252 100
253 20.1 17.8 26.6
125 12.7 7.7 11.5#

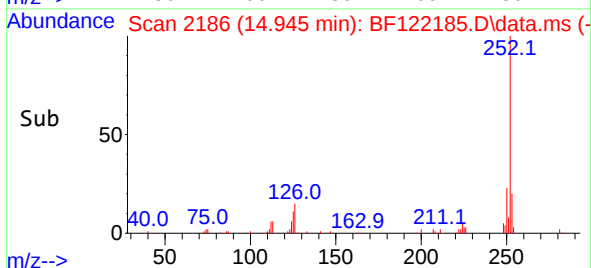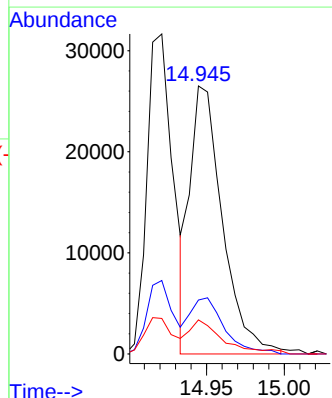







#90
Benzo(a)pyrene
Concen: 2.83 ng
RT: 15.268 min Scan# 2241
Delta R.T. 0.017 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:	252	Resp:	40195
Ion Ratio	Lower	Upper	
252	100		
253	23.1	17.3	25.9
125	11.6	8.6	13.0

Instrument :
BNA_F
ClientSampleId :
IB1-TREATED-EFFLU




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:05 PM

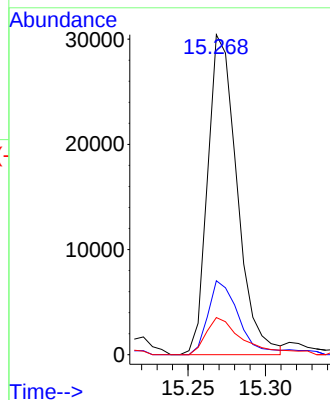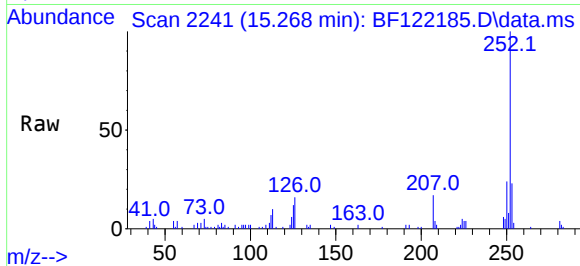

#91
Dibenzo(a,h)anthracene
Concen: 7.06 ng
RT: 16.745 min Scan# 2492
Delta R.T. 0.029 min
Lab File: BF122185.D
Acq: 30 Oct 2020 17:42

Tgt Ion:	278	Resp:	91859
Ion Ratio	Lower	Upper	
278	100		
139	16.0	13.0	19.4
279	22.6	19.0	28.4

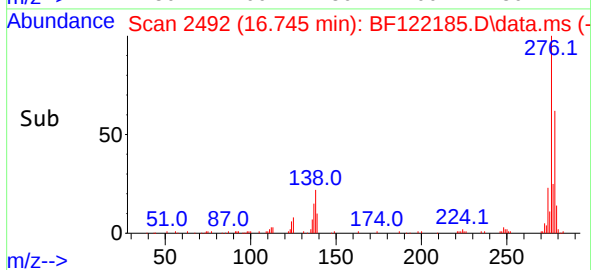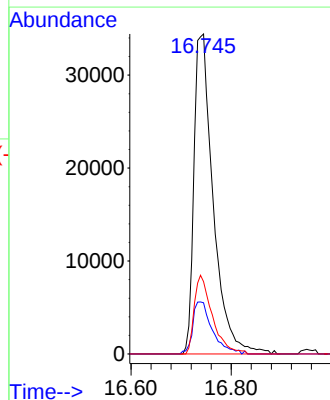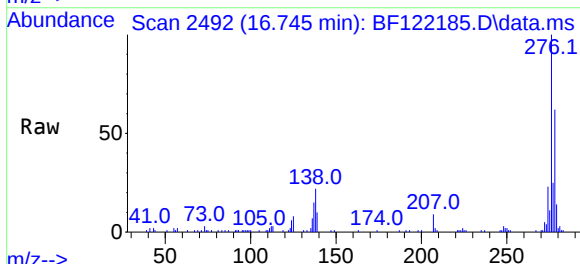



#92
 Benzo(g,h,i)perylene
 Concen: 9.36 ng
 RT: 17.174 min Scan# 2565
 Delta R.T. 0.041 min
 Lab File: BF122185.D
 Acq: 30 Oct 2020 17:42

Tgt Ion: 276 Resp: 121903

Ion	Ratio	Lower	Upper
276	100		
277	24.6	19.4	29.2
138	19.4	17.8	26.6

Instrument :
 BNA_F
 ClientSampleId :
 IB1-TREATED-EFFLU

Manual Integrations
 APPROVED

mohammad
 11/2/2020 12:36:05 PM

