

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122198.D
 Acq On : 31 Oct 2020 00:27
 Operator : JU/CG
 Sample : L4541-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 124031

Manual Integrations
 APPROVED

mohammad
 11/2/2020 12:36:30 PM

Quant Time: Oct 31 03:03:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 30 10:16:54 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.710	152	96059	20.00	ng	0.00
21) Naphthalene-d8	7.992	136	368057	20.00	ng	0.00
39) Acenaphthene-d10	9.745	164	174631	20.00	ng	0.00
64) Phenanthrene-d10	11.233	188	274501	20.00	ng	0.00
76) Chrysene-d12	13.880	240	198857	20.00	ng	0.00
86) Perylene-d12	15.315	264	211396	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	754804	115.97	ng	0.00
7) Phenol-d6	6.369	99	935562	111.67	ng	0.00
23) Nitrobenzene-d5	7.281	82	611072	85.15	ng	0.00
42) 2,4,6-Tribromophenol	10.539	330	226906	105.04	ng	0.00
45) 2-Fluorobiphenyl	9.069	172	917801	77.33	ng	0.00
79) Terphenyl-d14	12.816	244	645354	61.85	ng	0.00
Target Compounds						
						Qvalue
10) Phenol	6.381	94	57933	6.70	ng	92
50) Dimethylphthalate	9.469	163	191722	15.01	ng	99
71) Phenanthrene	11.257	178	57182	3.80	ng	98
75) Fluoranthene	12.451	202	133422	8.27	ng	97
78) Pyrene	12.680	202	117852	7.78	ng	97
81) Benzo(a)anthracene	13.868	228	65958	5.06	ng	97
83) Chrysene	13.910	228	59077	4.62	ng	98
87) Indeno(1,2,3-cd)pyrene	16.745	276	35122	2.56	ng	96
88) Benzo(b)fluoranthene	14.909	252	84194m	5.89	ng	
89) Benzo(k)fluoranthene	14.933	252	27294m	2.01	ng	
90) Benzo(a)pyrene	15.262	252	58549	4.74	ng	98
92) Benzo(g,h,i)perylene	17.174	276	33932	3.00	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122198.D
Acq On : 31 Oct 2020 00:27
Operator : JU/CG
Sample : L4541-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
124031

Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:30 PM

Quant Time: Oct 31 03:03:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration



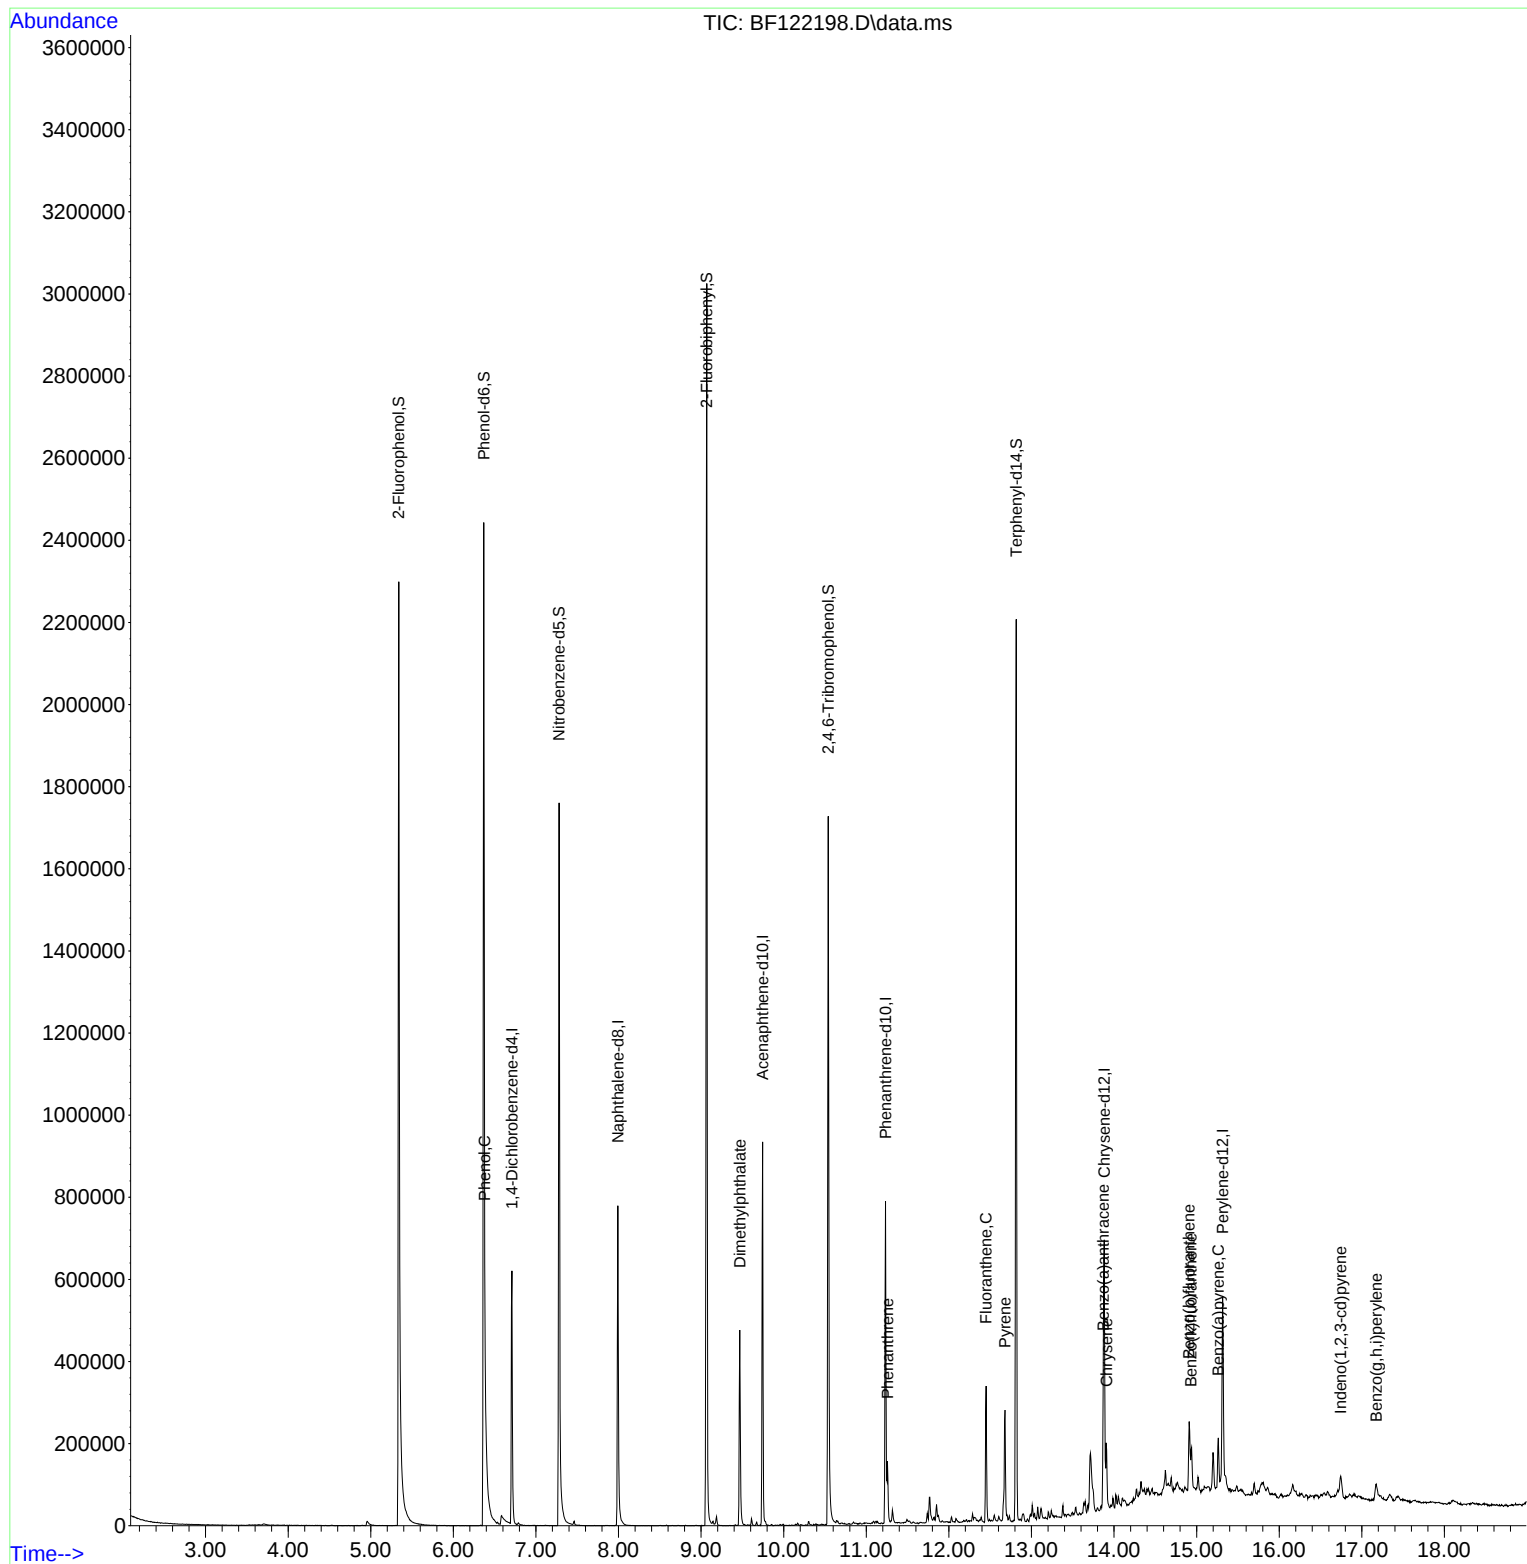





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.710 min Scan# 786
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

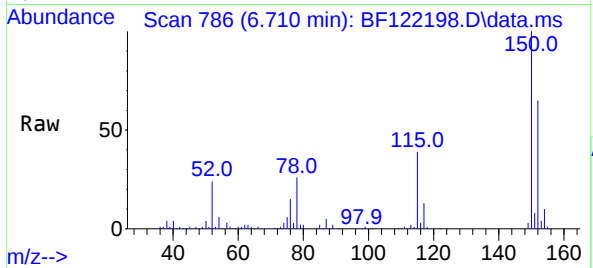



Tgt Ion:152 Resp: 96059
Ion Ratio Lower Upper
152 100
150 154.2 125.3 187.9
115 60.4 51.9 77.9

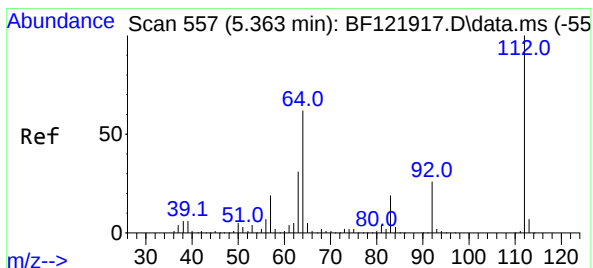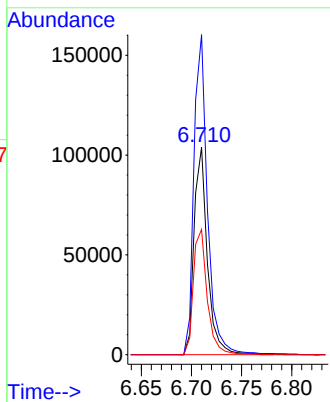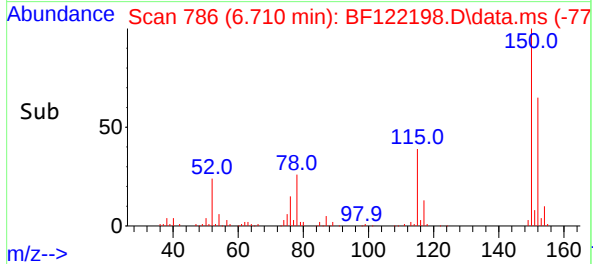

#5
2-Fluorophenol
Concen: 115.97 ng
RT: 5.340 min Scan# 553
Delta R.T. 0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

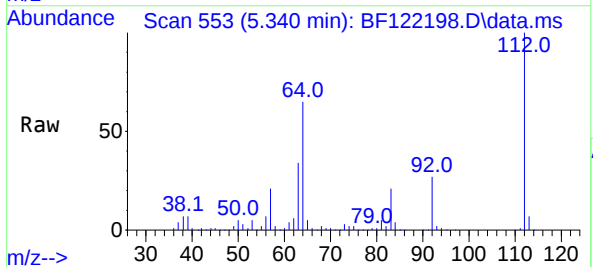

Tgt Ion:112 Resp: 754804
Ion Ratio Lower Upper
112 100
64 65.4 50.4 75.6
63 33.9 25.8 38.6

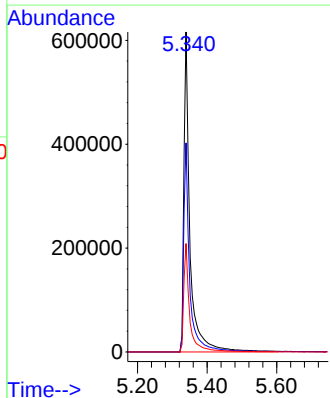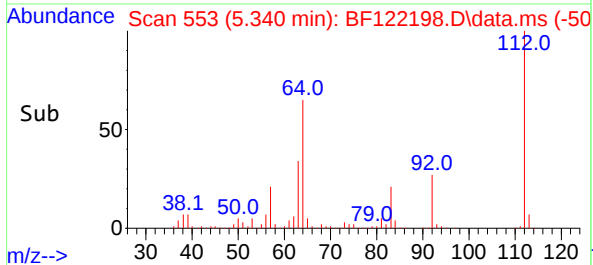

Instrument :
BNA_F
ClientSampleId :
124031

Manual Integrations
APPROVED

mohammad
11/2/2020 12:36:30 PM







#7
Phenol-d6
Concen: 111.67 ng
RT: 6.369 min Scan# 728
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion: 99 Resp: 935562
Ion Ratio Lower Upper
99 100
42 21.5 15.9 23.9
71 37.5 27.1 40.7

Instrument :
BNA_F
ClientSampled :
124031




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:30 PM

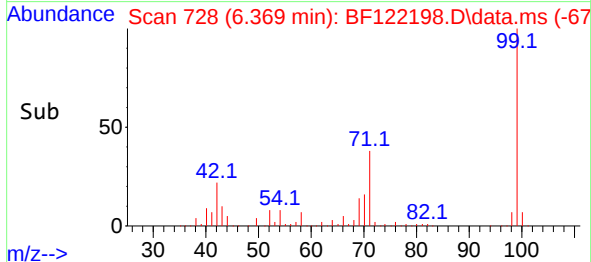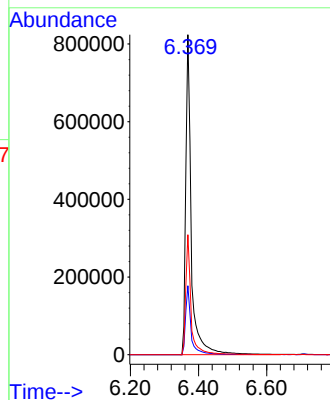


#10
Phenol
Concen: 6.70 ng
RT: 6.381 min Scan# 730
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion: 94 Resp: 57933
Ion Ratio Lower Upper
94 100
65 32.8 17.1 57.1
66 62.4 36.0 76.0

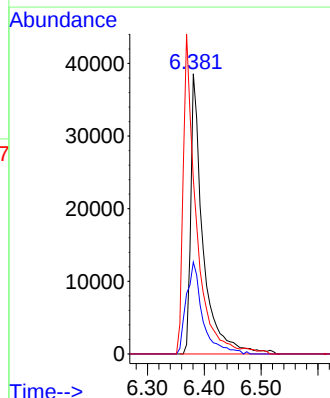





#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.992 min Scan# 1004
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27




Tgt Ion:136 Resp: 368057
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 9.2 7.1 10.7
68 6.2 5.0 7.4

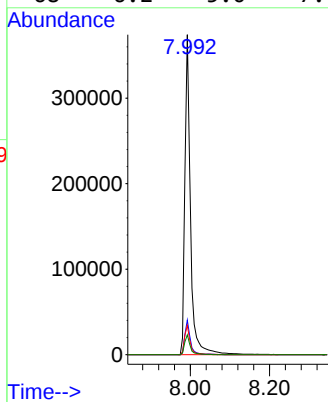


Instrument :
BNA_F
ClientSampled :
124031

Manual Integrations
APPROVED



mohammad
11/2/2020 12:36:30 PM




#23
Nitrobenzene-d5
Concen: 85.15 ng
RT: 7.281 min Scan# 883
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27




Tgt Ion: 82 Resp: 611072
Ion Ratio Lower Upper
82 100
128 41.1 35.0 52.4
54 55.2 43.9 65.9


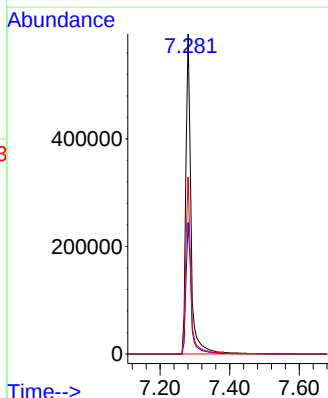






#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.745 min Scan# 1302
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27





Tgt Ion:164 Resp: 174631
Ion Ratio Lower Upper
164 100
162 102.4 83.2 124.8
160 47.2 37.5 56.3

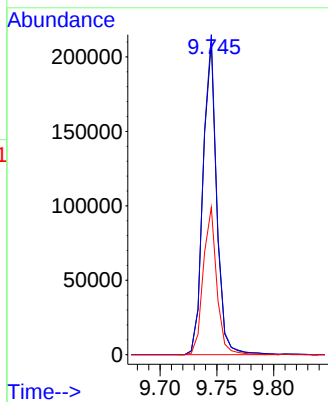

#42
2,4,6-Tribromophenol
Concen: 105.04 ng
RT: 10.539 min Scan# 1437
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

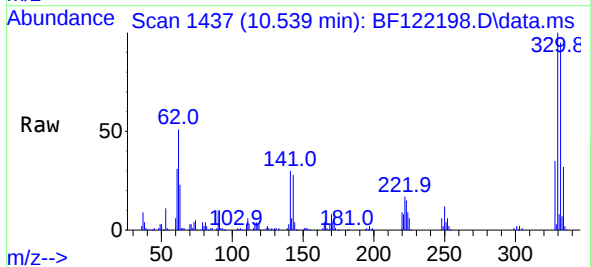


Tgt Ion:330 Resp: 226906
Ion Ratio Lower Upper
330 100
332 96.0 77.3 115.9
141 30.2 22.3 33.5

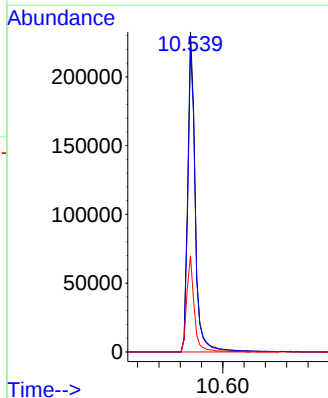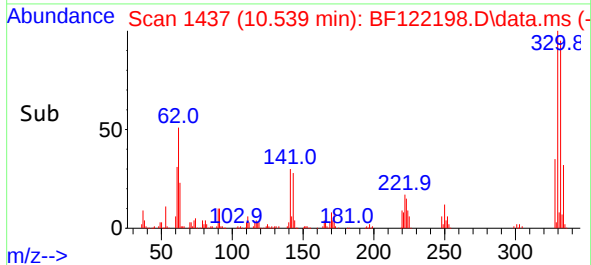

Instrument :
BNA_F
ClientSampleId :
124031


Manual Integrations
APPROVED

mohammad
11/2/2020 12:36:30 PM



#45
2-Fluorobiphenyl
Concen: 77.33 ng
RT: 9.069 min Scan# 1187
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27




Instrument :
BNA_F
ClientSampled :
124031




Tgt Ion:172 Resp: 917801
Ion Ratio Lower Upper
172 100
171 36.3 29.1 43.7
170 24.1 19.8 29.6

Manual Integrations
APPROVED



mohammad
11/2/2020 12:36:30 PM

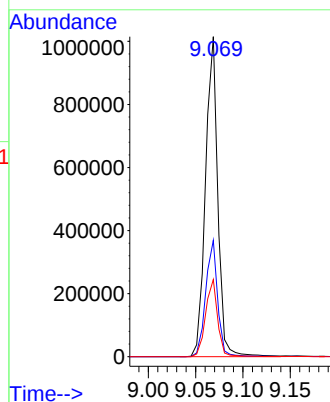


#50
Dimethylphthalate
Concen: 15.01 ng
RT: 9.469 min Scan# 1255
Delta R.T. -0.012 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27




Tgt Ion:163 Resp: 191722
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.0 8.2 12.4

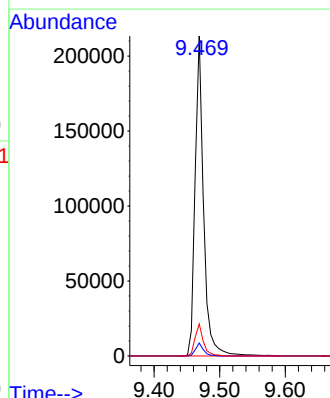



#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.233 min Scan# 1555
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27




Instrument :
BNA_F
ClientSampled :
124031




Tgt Ion:188 Resp: 274501
Ion Ratio Lower Upper
188 100
94 10.0 8.3 12.5
80 10.7 9.1 13.7

Manual Integrations
APPROVED



mohammad
11/2/2020 12:36:30 PM

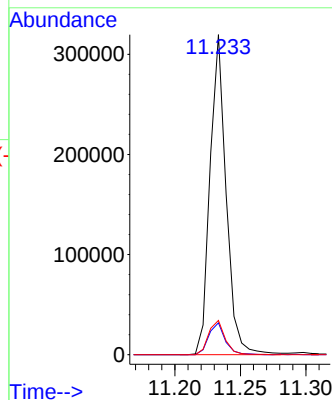


#71
Phenanthrene
Concen: 3.80 ng
RT: 11.257 min Scan# 1559
Delta R.T. -0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27



Tgt Ion:178 Resp: 57182
Ion Ratio Lower Upper
178 100
176 19.4 15.9 23.9
179 14.1 12.2 18.4

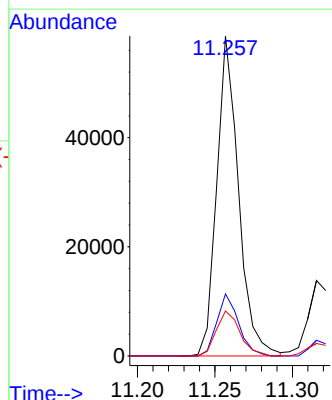







#75
Fluoranthene
Concen: 8.27 ng
RT: 12.451 min Scan# 1762
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:	202	Resp:	133422
Ion Ratio	Lower	Upper	
202	100		
101	10.7	0.0	33.4
203	17.7	0.0	37.9

Instrument :
BNA_F
ClientSampleId :
124031




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:30 PM

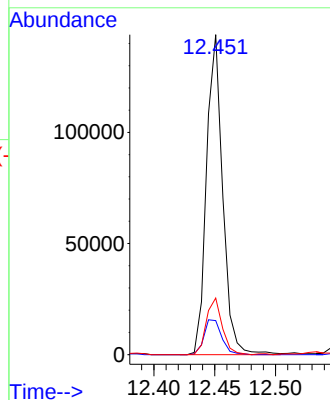

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.880 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:	240	Resp:	198857
Ion Ratio	Lower	Upper	
240	100		
120	10.6	9.2	13.8
236	25.4	20.9	31.3

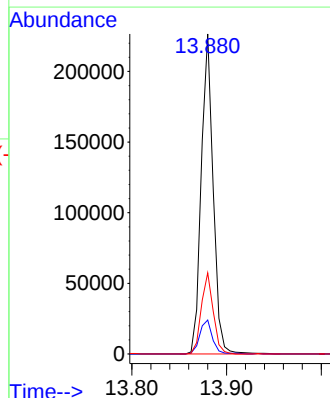







#78
Pyrene
Concen: 7.78 ng
RT: 12.680 min Scan# 1801
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:202 Resp: 117852
Ion Ratio Lower Upper
202 100
200 21.0 17.4 26.2
203 15.9 14.6 21.8

Instrument :
BNA_F
ClientSampleId :
124031




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:30 PM

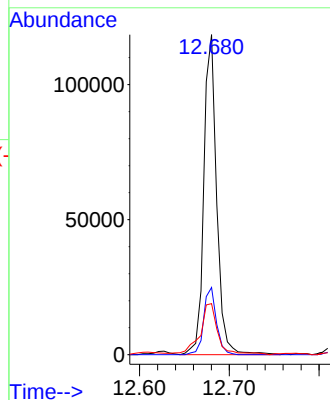

#79
Terphenyl-d14
Concen: 61.85 ng
RT: 12.816 min Scan# 1824
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:244 Resp: 645354
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.2
122 10.6 8.1 12.1

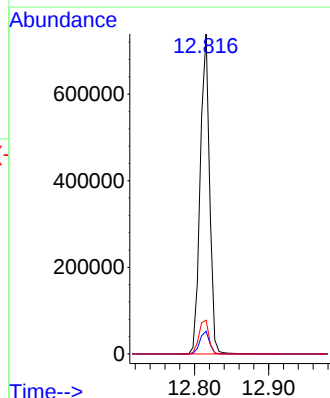







#81
Benzo(a)anthracene
Concen: 5.06 ng
RT: 13.868 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:228 Resp: 65958
Ion Ratio Lower Upper
228 100
226 26.7 22.3 33.5
229 21.7 16.2 24.4

Instrument :
BNA_F
ClientSampleId :
124031




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:30 PM

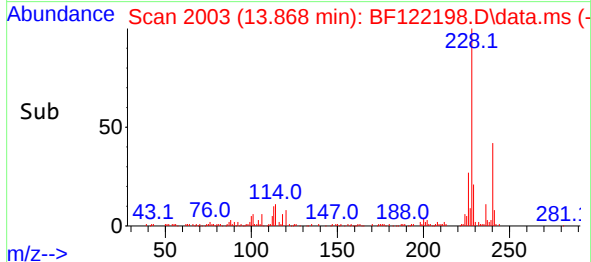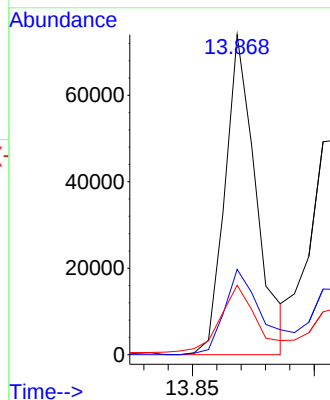


#83
Chrysene
Concen: 4.62 ng
RT: 13.910 min Scan# 2010
Delta R.T. 0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:228 Resp: 59077
Ion Ratio Lower Upper
228 100
226 30.4 24.6 37.0
229 21.6 15.9 23.9

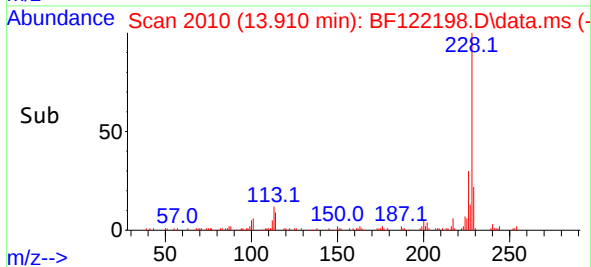
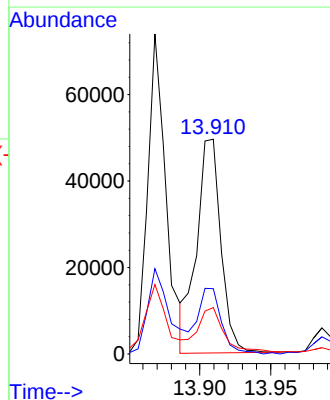
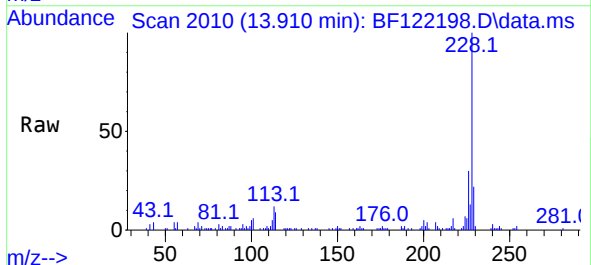





#86
Perylene-d12
Concen: 20.00 ng
RT: 15.315 min Scan# 2249
Delta R.T. 0.012 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27





Tgt Ion:264 Resp: 211396
Ion Ratio Lower Upper
264 100
260 23.5 18.7 28.1
265 21.7 17.3 25.9

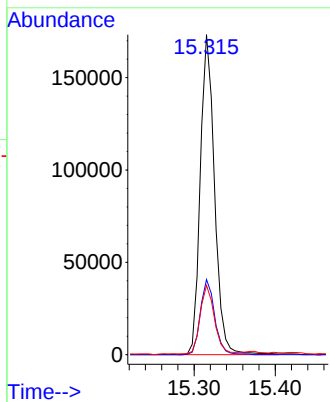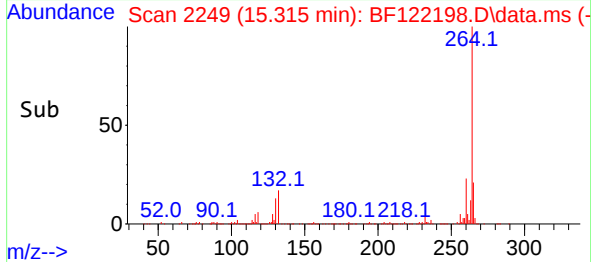

#87
Indeno(1,2,3-cd)pyrene
Concen: 2.56 ng
RT: 16.745 min Scan# 2492
Delta R.T. 0.029 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

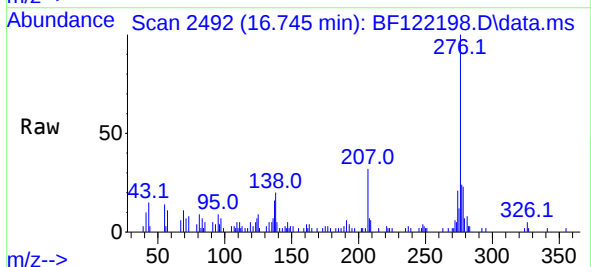


Tgt Ion:276 Resp: 35122
Ion Ratio Lower Upper
276 100
138 24.1 19.9 29.9
277 29.2 20.4 30.6

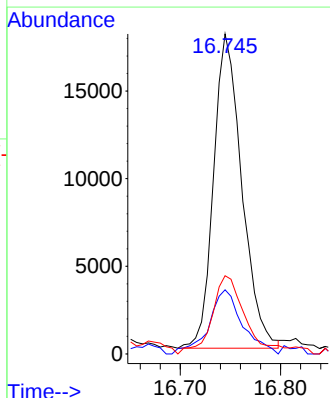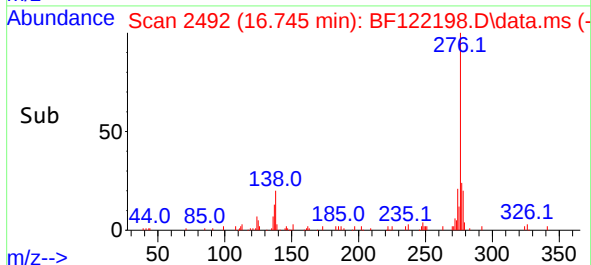

Instrument :
BNA_F
ClientSampleId :
124031

Manual Integrations
APPROVED

mohammad
11/2/2020 12:36:30 PM







#88
Benzo(b)fluoranthene
Concen: 5.89 ng m
RT: 14.909 min Scan# 2180
Delta R.T. 0.012 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:252 Resp: 84194
Ion Ratio Lower Upper
252 100
253 22.8 18.2 27.2
125 11.5 8.0 12.0

Instrument :
BNA_F
ClientSampled :
124031




Manual Integrations
APPROVED


mohammad
11/2/2020 12:36:30 PM

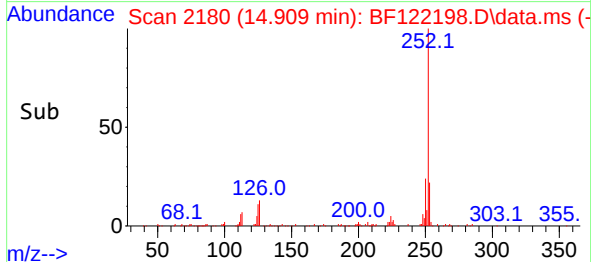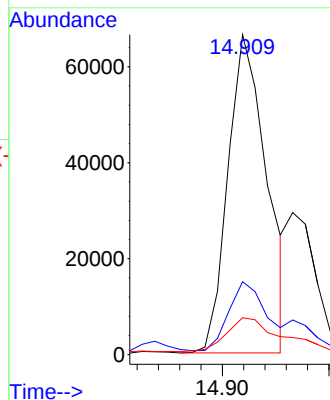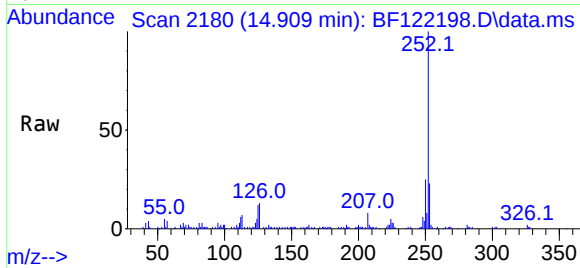

#89
Benzo(k)fluoranthene
Concen: 2.01 ng m
RT: 14.933 min Scan# 2184
Delta R.T. 0.006 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion:252 Resp: 27294
Ion Ratio Lower Upper
252 100
253 24.5 17.8 26.6
125 12.0 7.7 11.5#

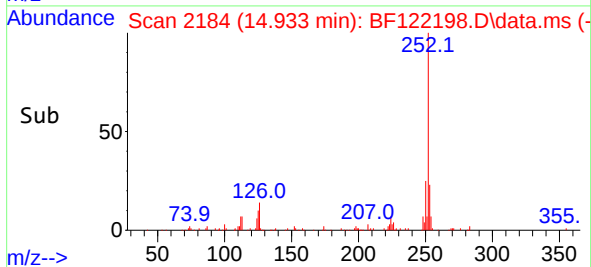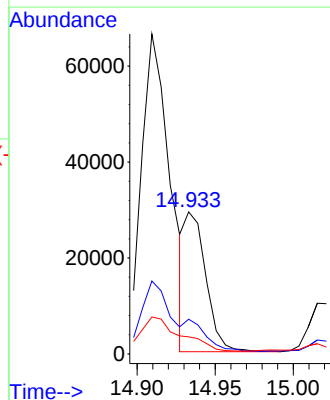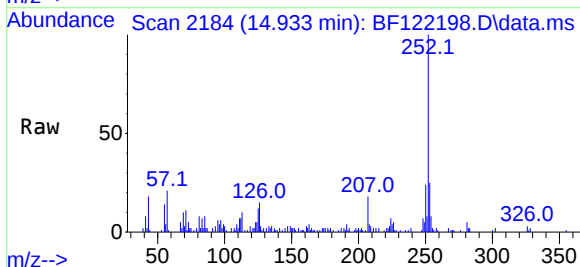







#90
Benzo(a)pyrene
Concen: 4.74 ng
RT: 15.262 min Scan# 2240
Delta R.T. 0.012 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion: 252 Resp: 58549
Ion Ratio Lower Upper
252 100
253 22.9 17.3 25.9
125 10.4 8.6 13.0

Instrument :
BNA_F
ClientSampled :
124031

Manual Integrations
APPROVED

mohammad
11/2/2020 12:36:30 PM

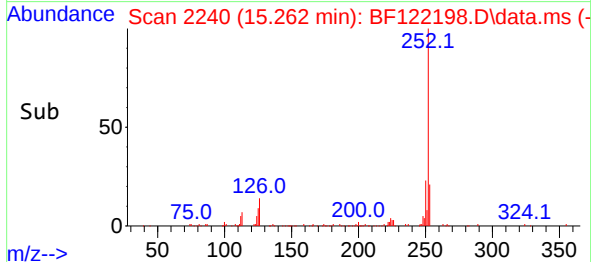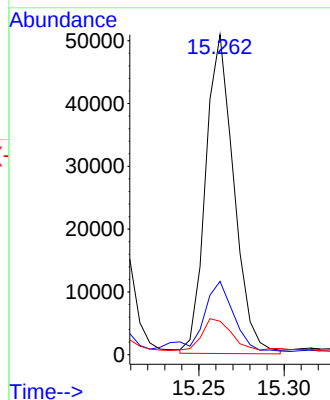

#92
Benzo(g,h,i)perylene
Concen: 3.00 ng
RT: 17.174 min Scan# 2565
Delta R.T. 0.041 min
Lab File: BF122198.D
Acq: 31 Oct 2020 00:27

Tgt Ion: 276 Resp: 33932
Ion Ratio Lower Upper
276 100
277 24.5 19.4 29.2
138 20.1 17.8 26.6

