

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122202.D
 Acq On : 31 Oct 2020 2:30
 Operator : JU/CG
 Sample : L4215-01 2X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AU-05-102820

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.340	550	553	579	rBV	588947	1036258	85.61%	10.338%
2	6.369	725	728	755	rBV	680575	1116938	92.28%	11.142%
3	6.710	782	786	798	rBV	632693	632138	52.23%	6.306%
4	7.281	880	883	902	rBV	570917	670959	55.43%	6.693%
5	7.992	1001	1004	1026	rBV	827727	803323	66.37%	8.014%
6	9.063	1183	1186	1198	rBV	1318852	1210394	100.00%	12.075%
7	9.469	1252	1255	1270	rVB	94639	108636	8.98%	1.084%
8	9.745	1298	1302	1313	rBV	883870	804110	66.43%	8.022%
9	10.539	1434	1437	1452	rBV	491325	538966	44.53%	5.377%
10	11.233	1551	1555	1565	rBV	699939	653710	54.01%	6.521%
11	11.763	1642	1645	1652	rBV3	11108	17239	1.42%	0.172%
12	12.304	1733	1737	1739	rBV	24618	22655	1.87%	0.226%
13	12.815	1820	1824	1830	rBV	972303	881751	72.85%	8.796%
14	13.727	1974	1979	1991	rBV3	55478	125950	10.41%	1.256%
15	13.880	2001	2005	2016	rBV	650998	678745	56.08%	6.771%
16	14.151	2047	2051	2054	rBV5	10653	16062	1.33%	0.160%
17	14.327	2077	2081	2085	rBV6	20871	32167	2.66%	0.321%
18	14.692	2140	2143	2147	rBV	63413	57836	4.78%	0.577%
19	15.315	2245	2249	2261	rVB	475643	616391	50.92%	6.149%




Sum of corrected areas: 10024228

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122202.D
Acq On : 31 Oct 2020 2:30
Operator : JU/CG
Sample : L4215-01 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AU-05-102820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

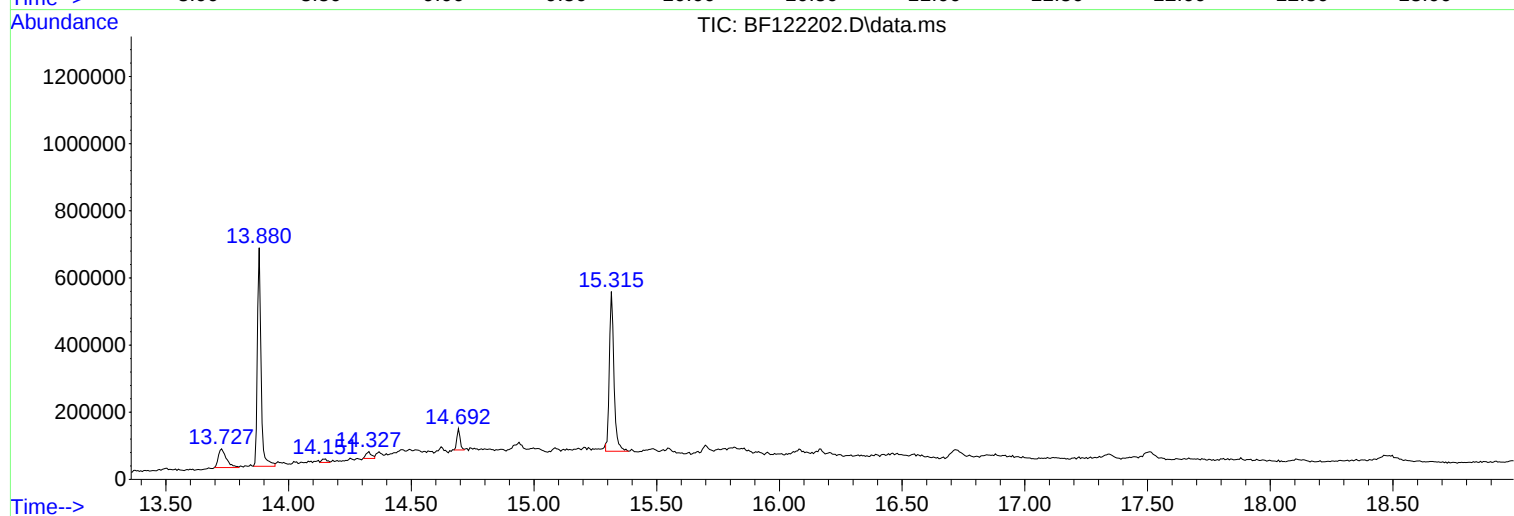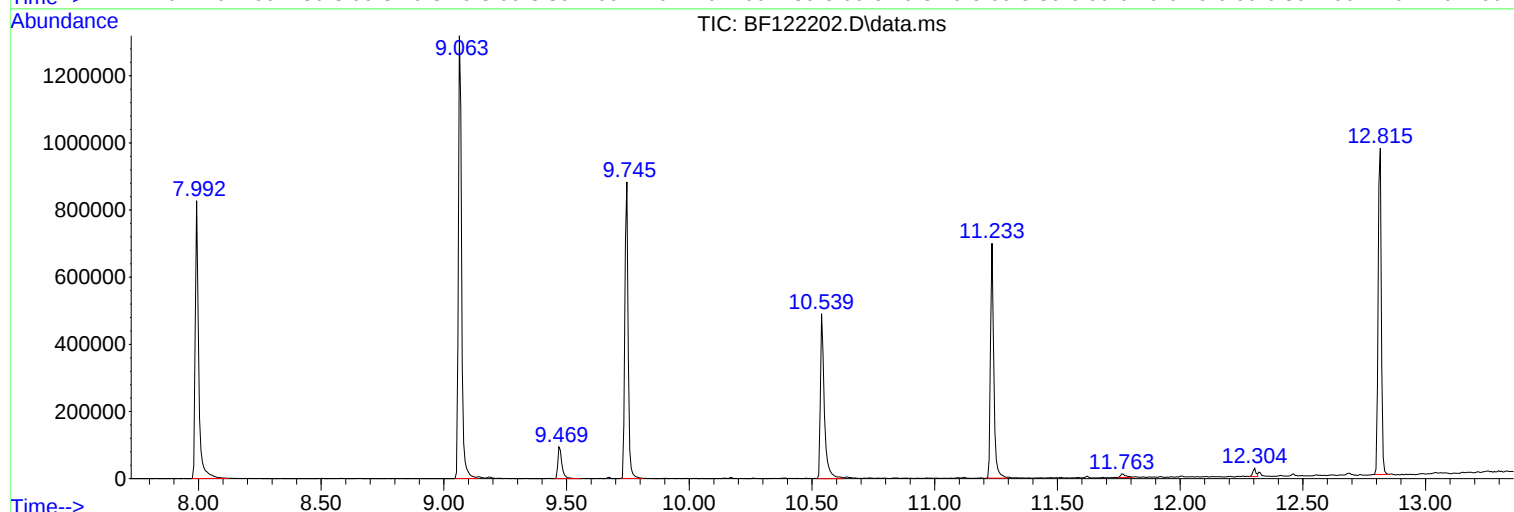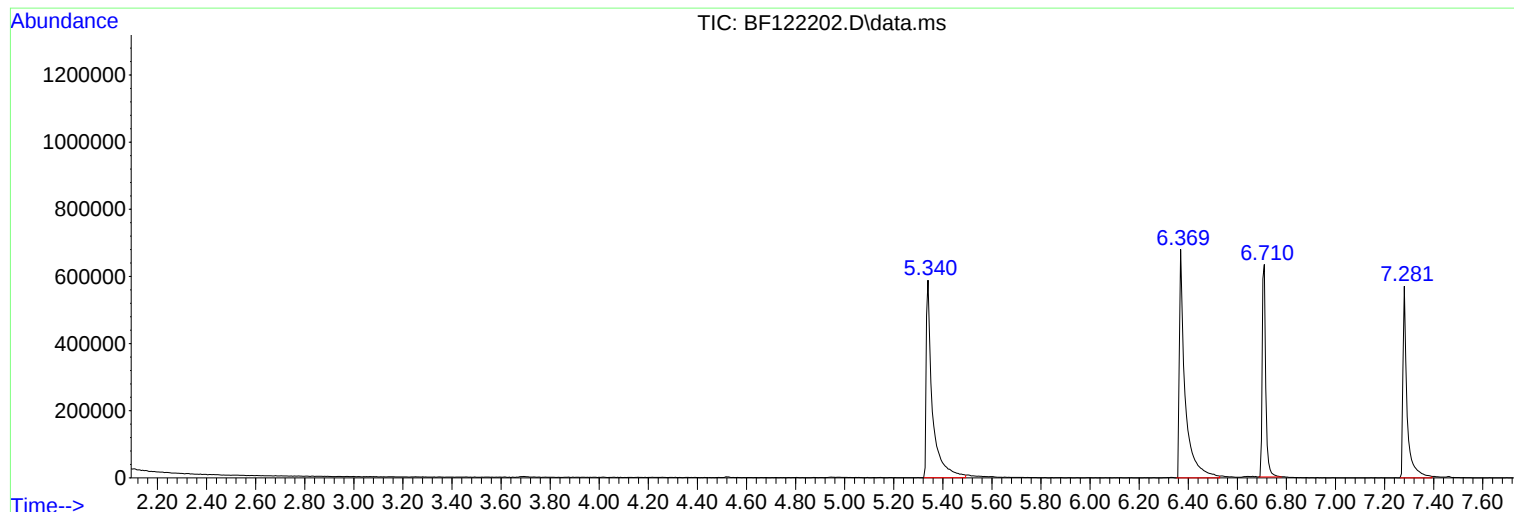

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122202.D
Acq On : 31 Oct 2020 2:30
Operator : JU/CG
Sample : L4215-01 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AU-05-102820










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentafluoropropionic acid, ... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.727	3.71 ng	125950	Chrysene-d12	13.880

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	95
2			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	95
3			2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	94
4			2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	94
5			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	93

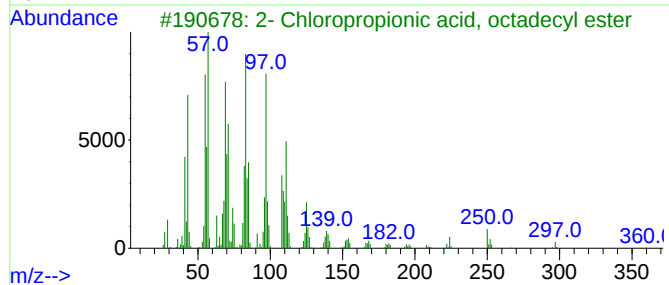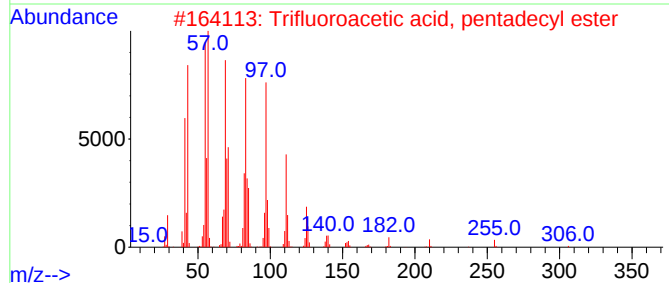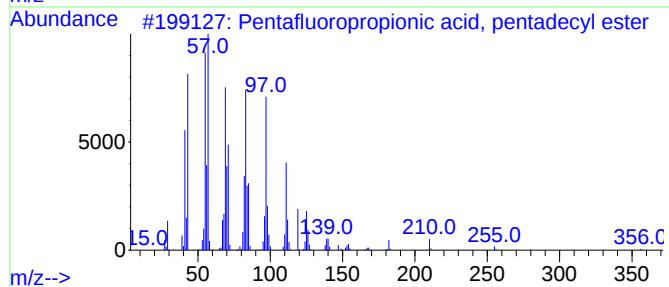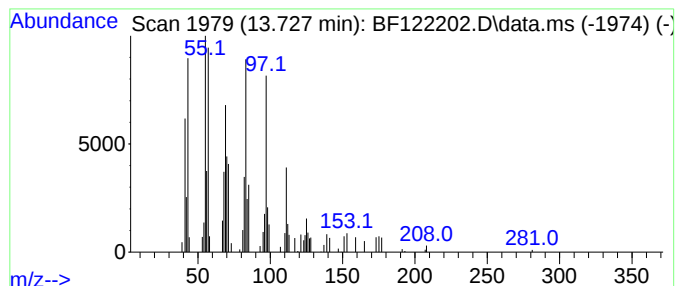

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122202.D
Acq On : 31 Oct 2020 2:30
Operator : JU/CG
Sample : L4215-01 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AU-05-102820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentafluoroprop...	13.727	3.7	ng	125950	5	13.880	678745	20.0