

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122204.D
 Acq On : 31 Oct 2020 3:32
 Operator : JU/CG
 Sample : L4217-07 2X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-01-102820

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	549	552	578	rBV	781349	1255936	92.10%	11.469%
2	6.369	725	728	754	rBV	865128	1363632	100.00%	12.452%
3	6.710	783	786	797	rBV	652529	633581	46.46%	5.786%
4	7.281	880	883	903	rBV	734301	822777	60.34%	7.513%
5	7.992	1001	1004	1012	rBV	849655	761794	55.87%	6.956%
6	8.410	1071	1075	1077	rBV	16422	15364	1.13%	0.140%
7	8.451	1079	1082	1086	rBV5	9065	16021	1.17%	0.146%
8	9.063	1183	1186	1196	rVV	1350483	1306377	95.80%	11.929%
9	9.145	1196	1200	1204	rVB	18252	22729	1.67%	0.208%
10	9.469	1252	1255	1262	rVB	143243	138133	10.13%	1.261%
11	9.745	1298	1302	1311	rVB	901925	795039	58.30%	7.260%
12	10.386	1405	1411	1416	rBV2	11688	17483	1.28%	0.160%
13	10.539	1434	1437	1452	rBV	666435	683595	50.13%	6.242%
14	10.651	1452	1456	1459	rVB2	17717	27189	1.99%	0.248%
15	11.116	1533	1535	1541	rVB3	17124	19804	1.45%	0.181%
16	11.233	1551	1555	1564	rBV	771371	694463	50.93%	6.341%
17	11.763	1642	1645	1649	rBV4	11577	13930	1.02%	0.127%
18	12.292	1732	1735	1736	rBV2	13357	14274	1.05%	0.130%
19	12.310	1736	1738	1742	rVB2	25641	22570	1.66%	0.206%
20	12.404	1752	1754	1759	rVB5	13487	14522	1.06%	0.133%
21	12.457	1759	1763	1766	rBV	30969	37622	2.76%	0.344%
22	12.680	1798	1801	1807	rVB	66171	71084	5.21%	0.649%
23	12.733	1808	1810	1813	rBV3	13166	14354	1.05%	0.131%
24	12.816	1820	1824	1834	rVB	1183475	1028304	75.41%	9.390%
25	13.039	1860	1862	1864	rBV	21094	15292	1.12%	0.140%
26	13.380	1917	1920	1923	rBV2	40959	40395	2.96%	0.369%
27	13.880	2002	2005	2009	rBV	666983	617873	45.31%	5.642%
28	15.321	2247	2250	2257	rVB	385885	487039	35.72%	4.447%


Sum of corrected areas: 10951176

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122204.D
Acq On : 31 Oct 2020 3:32
Operator : JU/CG
Sample : L4217-07 2X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
HR-01-102820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

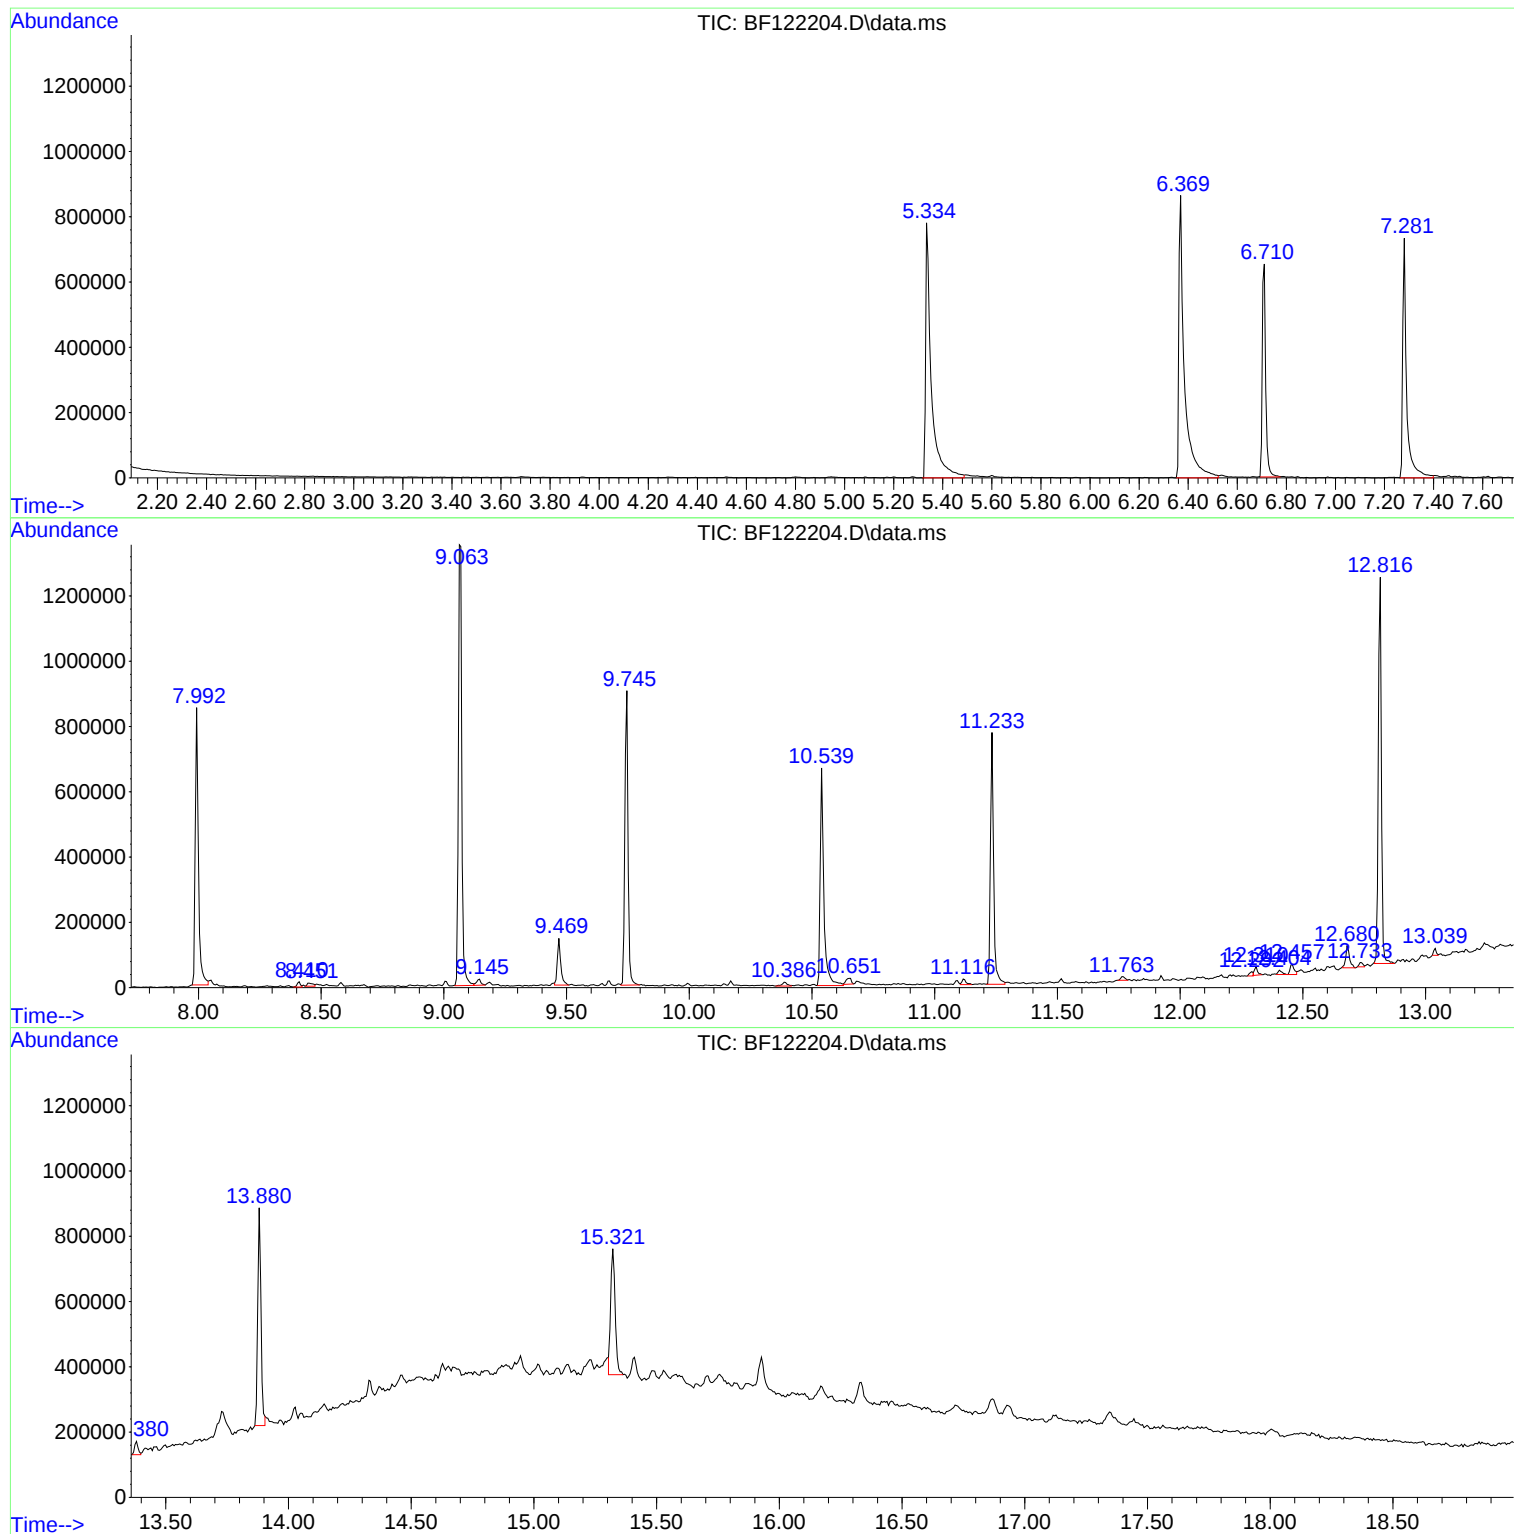

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122204.D
Acq On : 31 Oct 2020 3:32
Operator : JU/CG
Sample : L4217-07 2X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-01-102820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
Data File : BF122204.D
Acq On : 31 Oct 2020 3:32
Operator : JU/CG
Sample : L4217-07 2X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-01-102820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
