
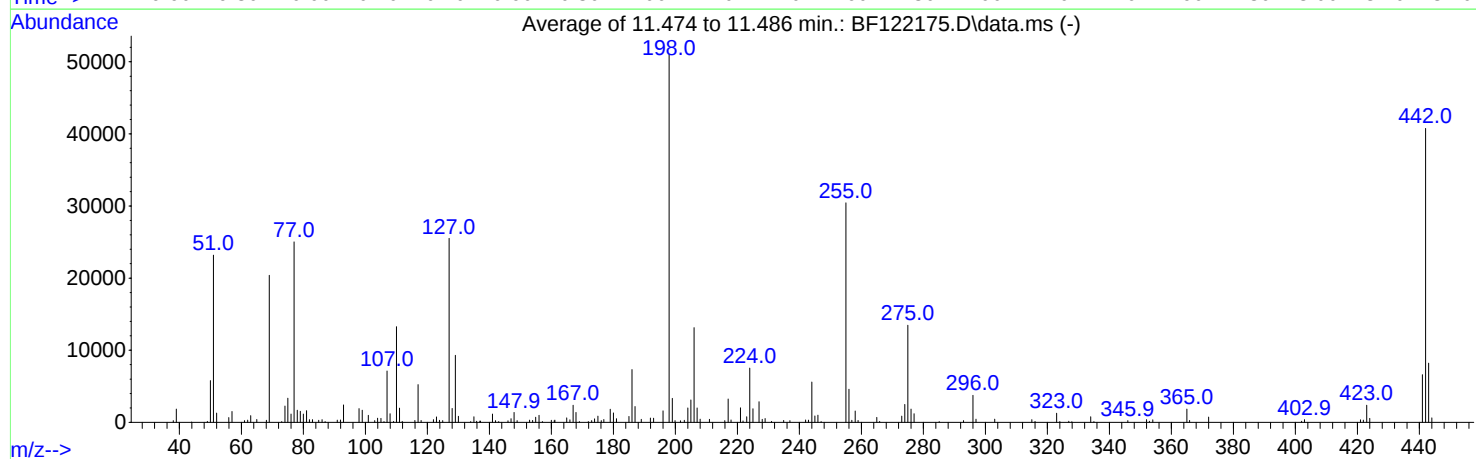


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122175.D
 Acq On : 30 Oct 2020 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 10:16:54 2020

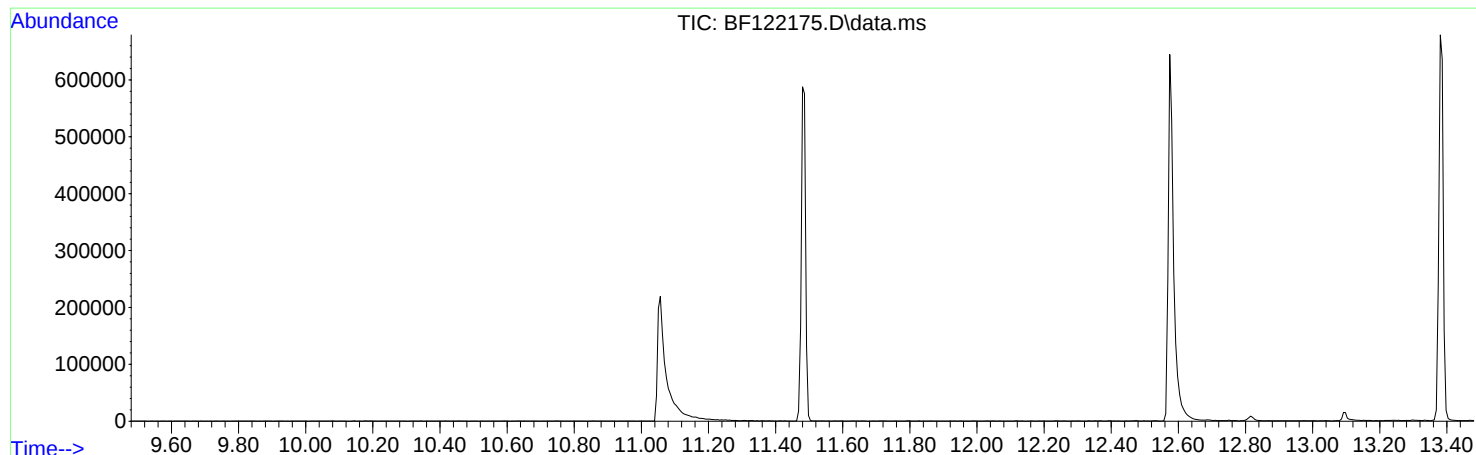

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	23195	PASS
68	69	0.00	2	1.4	282	PASS
69	198	0.00	100	40.0	20386	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	25508	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51008	PASS
199	198	5	9	6.5	3326	PASS
275	198	10	60	26.4	13466	PASS
365	198	1	100	3.6	1843	PASS
441	198	0.01	100	13.0	6607	PASS
442	198	50	100	79.9	40769	PASS
443	442	15	24	20.2	8216	PASS