
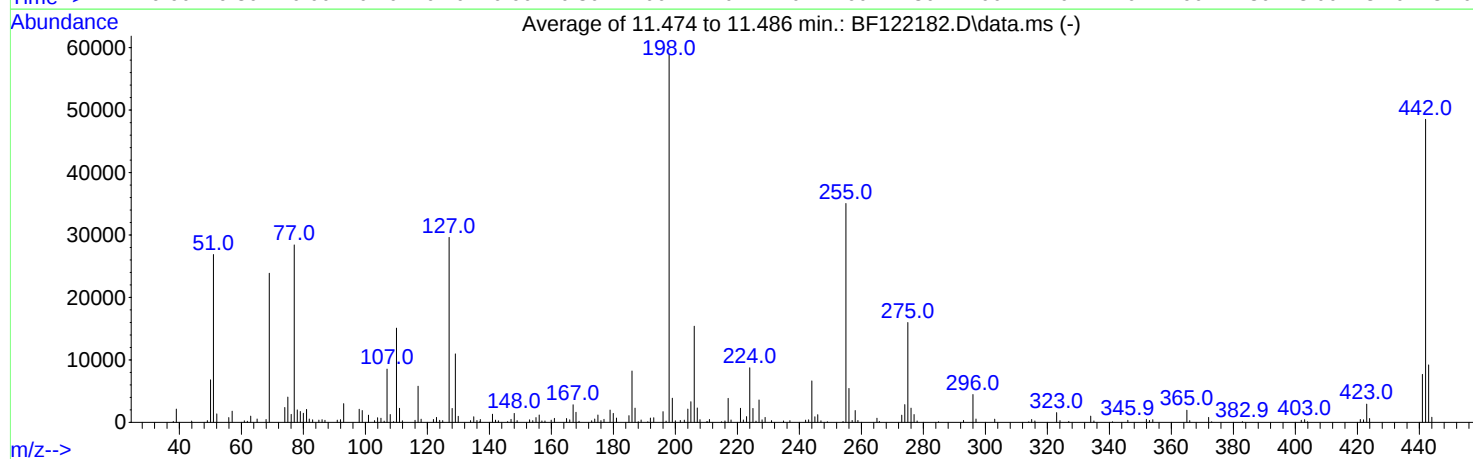


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122182.D
 Acq On : 30 Oct 2020 15:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 10:16:54 2020

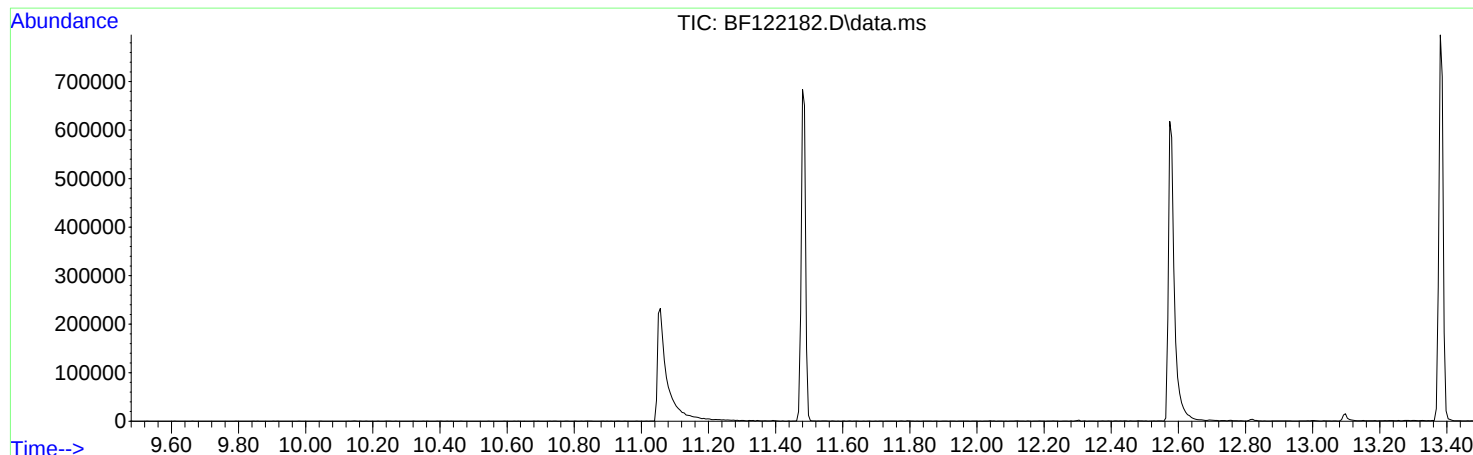

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	26867	PASS
68	69	0.00	2	2.0	466	PASS
69	198	0.00	100	40.6	23888	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	29617	PASS
197	198	0.00	2	0.4	219	PASS
198	198	100	100	100.0	58904	PASS
199	198	5	9	6.6	3859	PASS
275	198	10	60	27.2	15999	PASS
365	198	1	100	3.3	1954	PASS
441	198	0.01	100	13.1	7696	PASS
442	198	50	100	82.4	48522	PASS
443	442	15	24	19.0	9199	PASS