
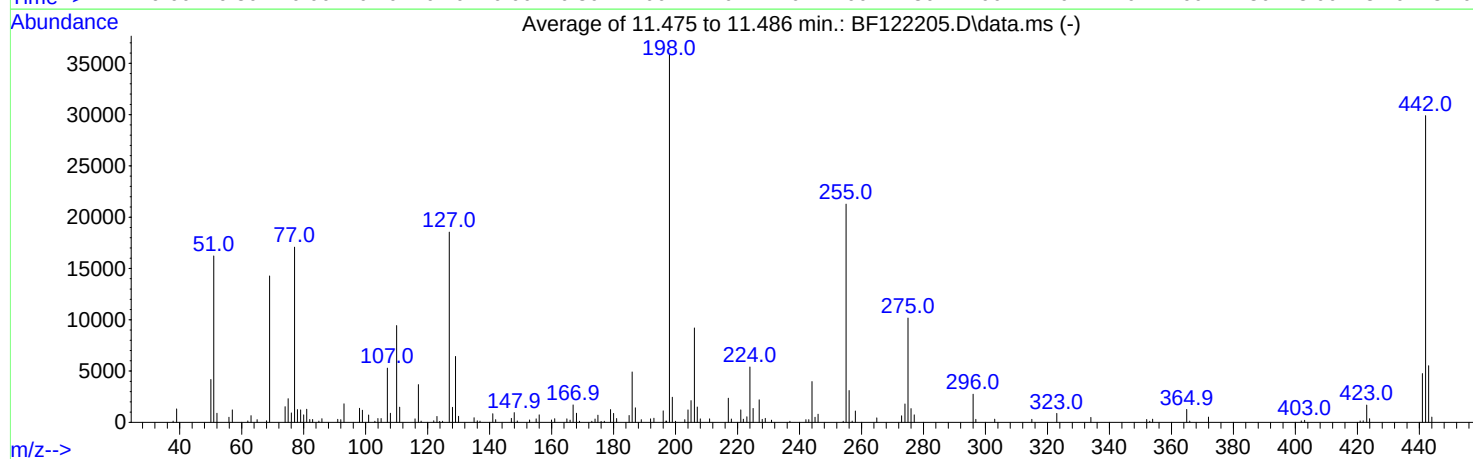


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103020\
 Data File : BF122205.D
 Acq On : 31 Oct 2020 5:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 10:16:54 2020

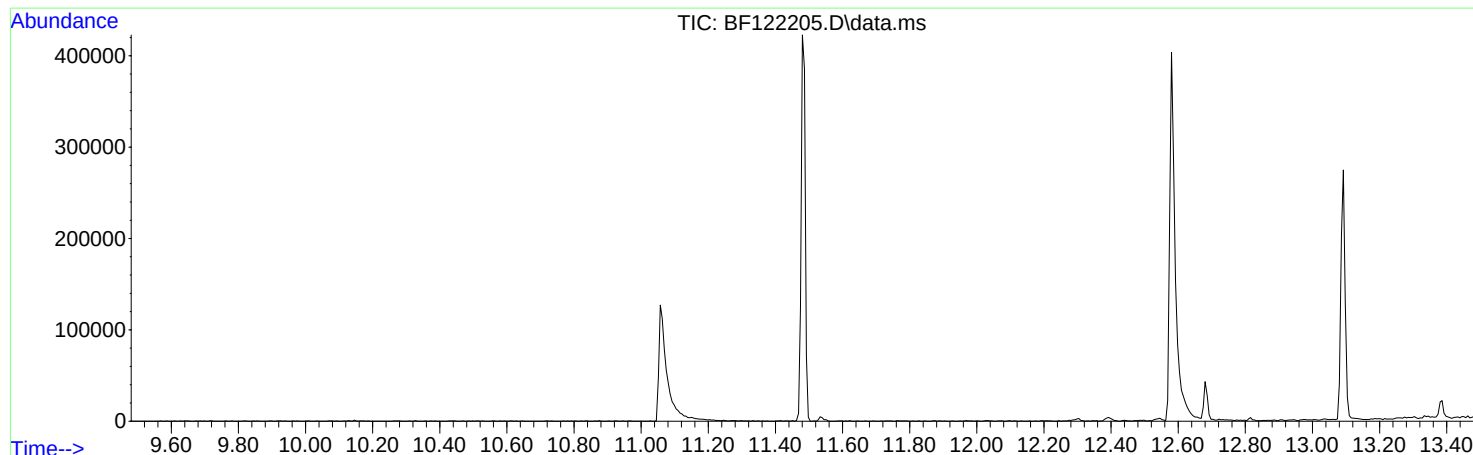

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	16226	PASS
68	69	0.00	2	1.1	163	PASS
69	198	0.00	100	39.8	14274	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	18543	PASS
197	198	0.00	2	0.3	124	PASS
198	198	100	100	100.0	35860	PASS
199	198	5	9	6.8	2455	PASS
275	198	10	60	28.4	10167	PASS
365	198	1	100	3.5	1263	PASS
441	198	0.01	100	13.3	4756	PASS
442	198	50	100	83.4	29901	PASS
443	442	15	24	18.5	5525	PASS