

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
 Data File : BF140162.D
 Acq On : 30 Oct 2024 17:20
 Operator : RC/JU
 Sample : P4611-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	5	12	19	rVB	901610	1440132	70.01%	9.374%
2	5.104	504	512	518	rVB2	16106	27538	1.34%	0.179%
3	5.498	573	579	584	rBV	1325779	1758136	85.47%	11.443%
4	6.498	743	749	755	rBV	1343662	1830070	88.96%	11.912%
5	6.881	809	814	819	rVB	462192	565100	27.47%	3.678%
6	7.440	903	909	914	rBV	965374	1224382	59.52%	7.969%
7	7.692	948	952	956	rBV	29895	35584	1.73%	0.232%
8	8.163	1027	1032	1037	rBV	579700	703991	34.22%	4.582%
9	9.239	1209	1215	1220	rBV	1659313	2057102	100.00%	13.389%
10	9.922	1326	1331	1336	rBV	580535	715988	34.81%	4.660%
11	10.639	1447	1453	1460	rBV	315276	391887	19.05%	2.551%
12	10.710	1460	1465	1476	rBV	786062	1019069	49.54%	6.633%
13	10.945	1497	1505	1515	rVB	49512	67470	3.28%	0.439%
14	11.416	1580	1585	1592	rBV	462158	587262	28.55%	3.822%
15	11.945	1669	1675	1695	rBV2	120363	219742	10.68%	1.430%
16	12.733	1804	1809	1822	rBV	22528	44353	2.16%	0.289%
17	13.004	1850	1855	1861	rBV	1106298	1442296	70.11%	9.388%
18	13.921	2006	2011	2018	rBV2	34210	97781	4.75%	0.636%
19	14.069	2031	2036	2047	rVB	399508	566042	27.52%	3.684%
20	15.586	2288	2294	2315	rBV	314862	569786	27.70%	3.709%




Sum of corrected areas: 15363711

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
Data File : BF140162.D
Acq On : 30 Oct 2024 17:20
Operator : RC/JU
Sample : P4611-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

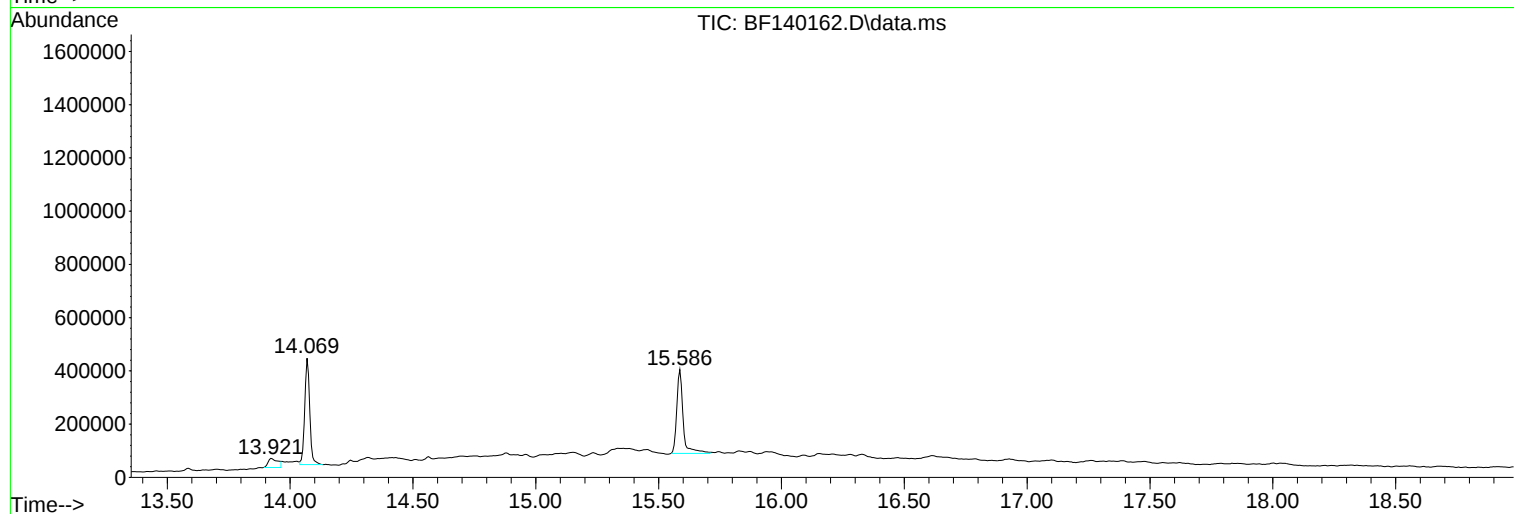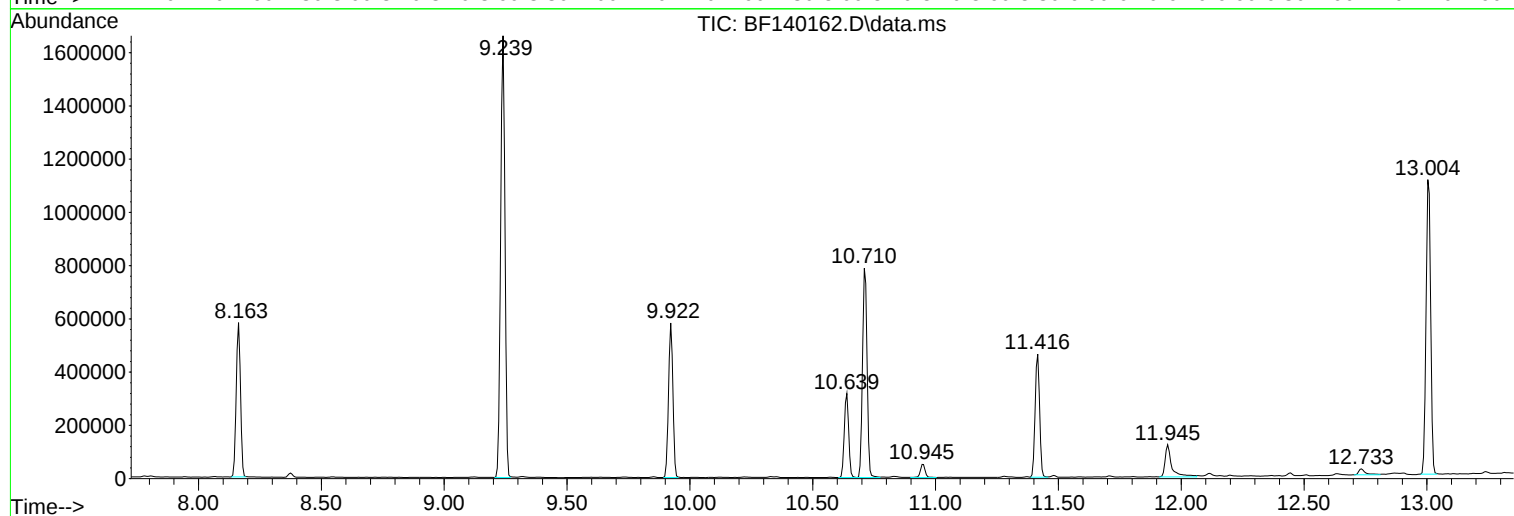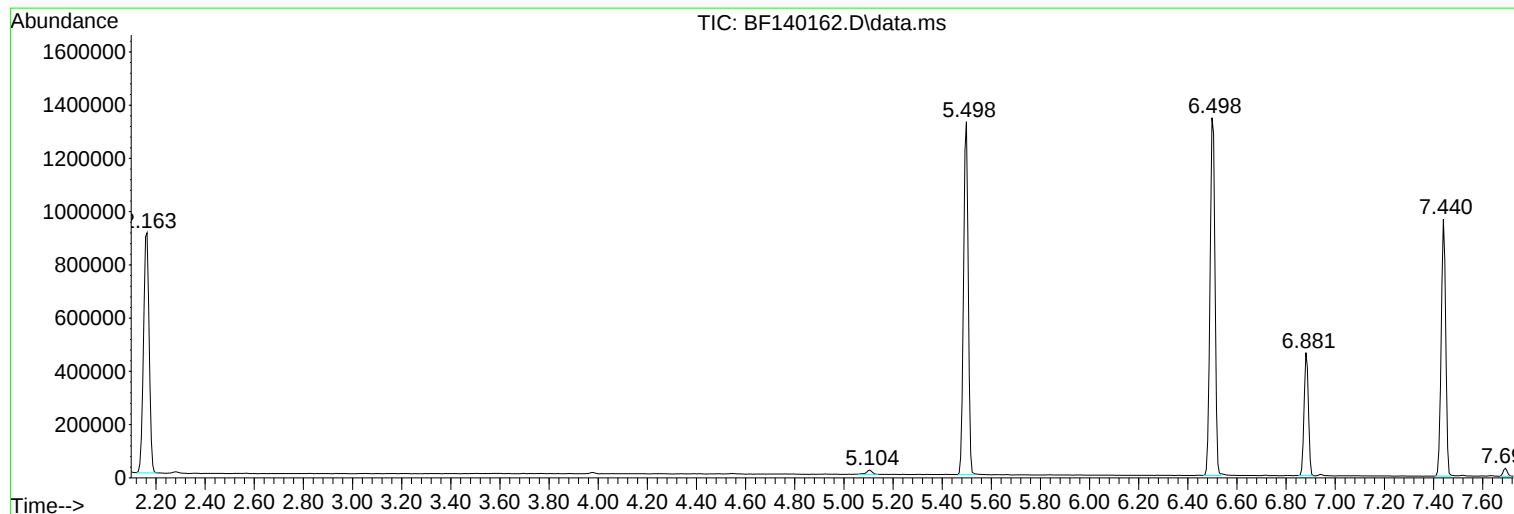

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
Data File : BF140162.D
Acq On : 30 Oct 2024 17:20
Operator : RC/JU
Sample : P4611-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
Data File : BF140162.D
Acq On : 30 Oct 2024 17:20
Operator : RC/JU
Sample : P4611-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc