

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103116\
 Data File : BF090929.D
 Acq On : 31 Oct 2016 15:44
 Operator : UM/SJ
 Sample : PB94407BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94407BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	245	247	257	rBV	554707	884041	15.06%	2.121%
2	5.356	283	286	288	rBV	3261170	4310568	73.41%	10.340%
3	6.396	374	377	380	rBV	3504403	3791547	64.57%	9.095%
4	6.521	385	388	390	rBV	4149213	4597705	78.30%	11.028%
5	6.750	405	408	410	rBV	865755	879536	14.98%	2.110%
6	6.899	419	421	424	rBV	2635407	3342032	56.92%	8.016%
7	7.310	455	457	460	rBV	2018356	2642173	45.00%	6.338%
8	8.030	518	520	523	rBV	1275625	1242059	21.15%	2.979%
9	9.116	612	615	617	rBV	4999699	5486334	93.44%	13.160%
10	9.779	671	673	676	rBV	1061427	1396671	23.79%	3.350%
11	10.202	707	710	713	rVB	36785	63021	1.07%	0.151%
12	10.579	740	743	745	rBV	2963650	3450559	58.77%	8.277%
13	11.265	801	803	806	rBV	1604905	1420598	24.19%	3.408%
14	12.853	939	942	945	rBV	4478884	5871589	100.00%	14.084%
15	13.905	1031	1034	1036	rBV	1063017	1334192	22.72%	3.200%
16	15.299	1153	1156	1159	rBV	823251	976815	16.64%	2.343%


Sum of corrected areas: 41689440

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103116\
Data File : BF090929.D
Acq On : 31 Oct 2016 15:44
Operator : UM/SJ
Sample : PB94407BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94407BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

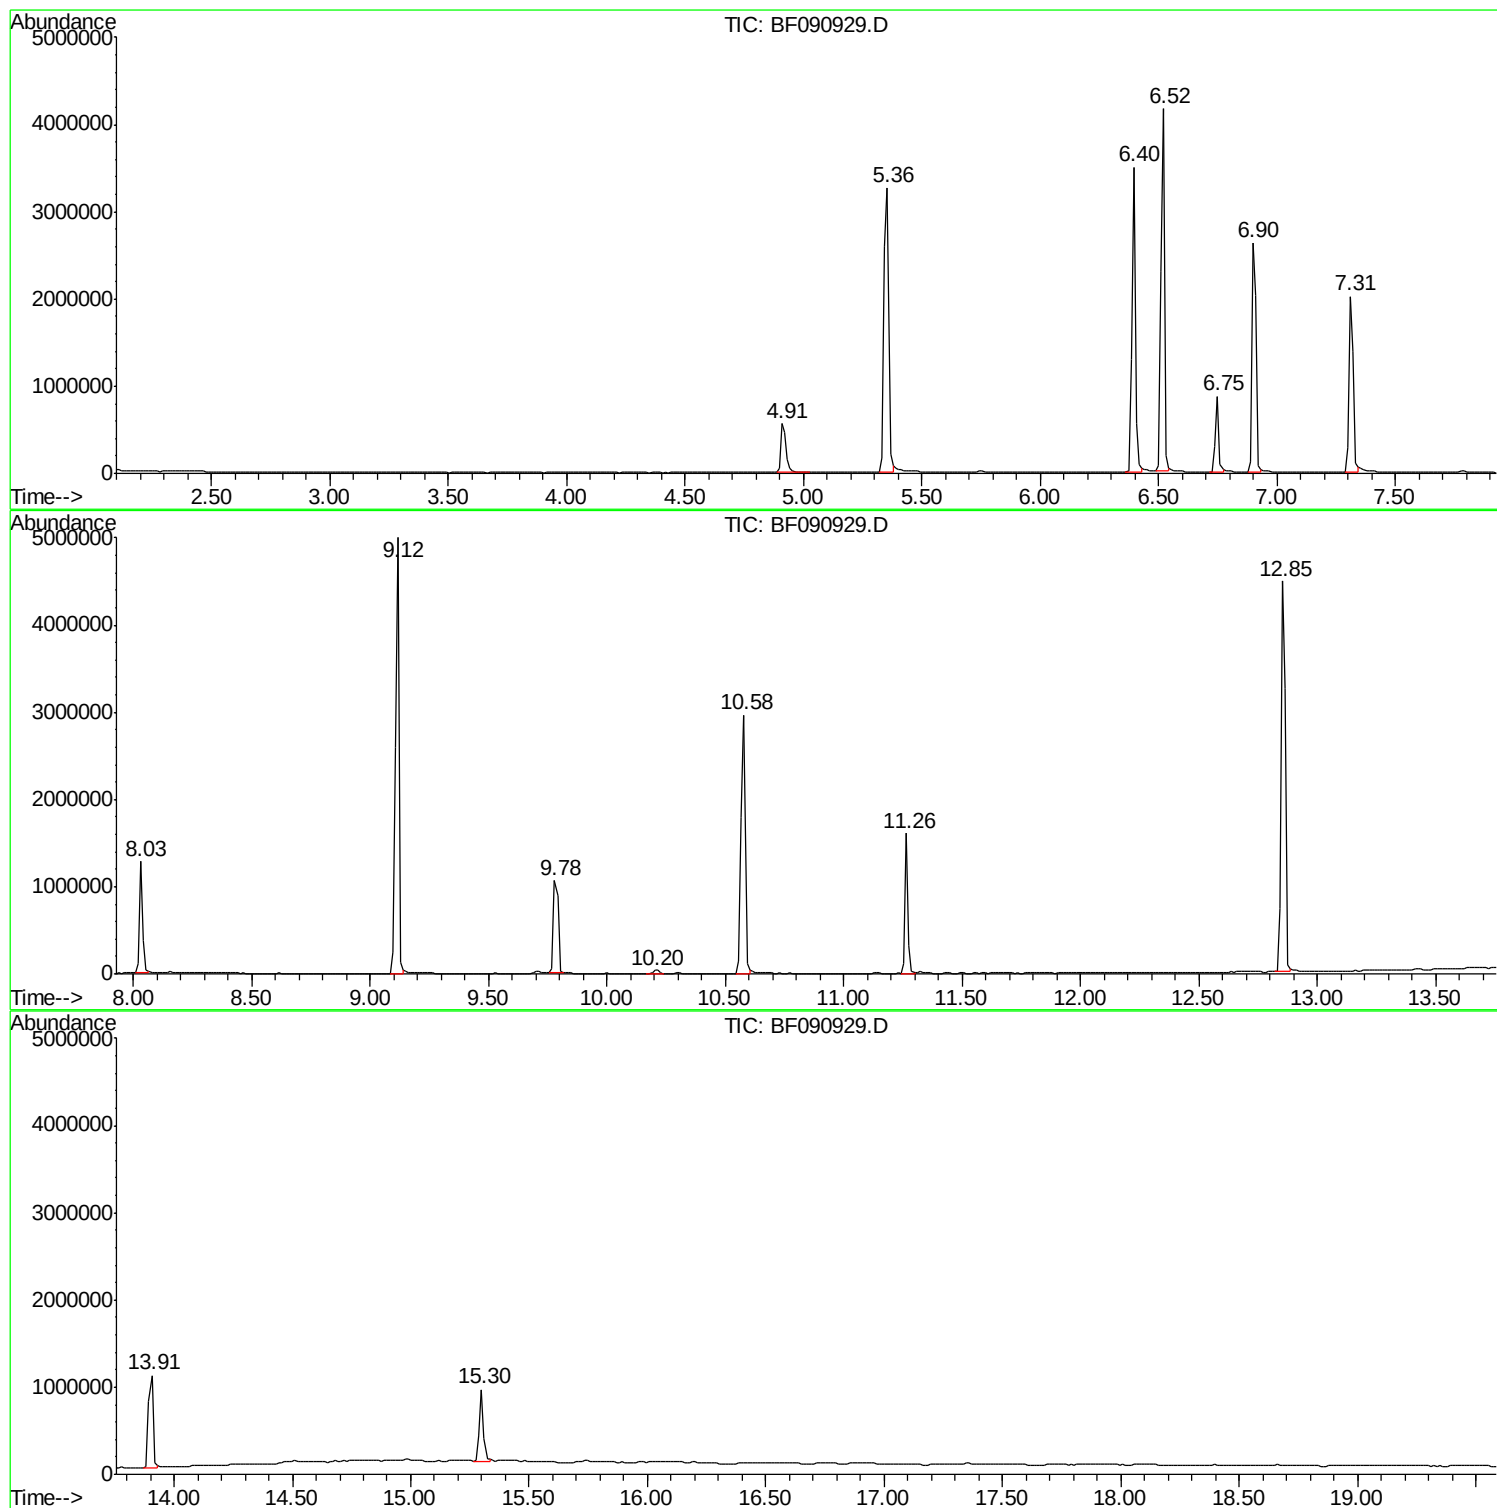

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103116\
Data File : BF090929.D
Acq On : 31 Oct 2016 15:44
Operator : UM/SJ
Sample : PB94407BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94407BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.91	20.10 ng	884041	1,4-Dichlorobenzene-d4	6.75

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	42
3		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28
4		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

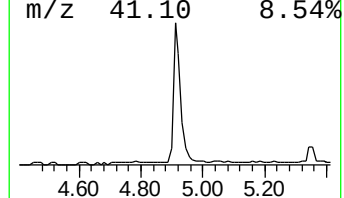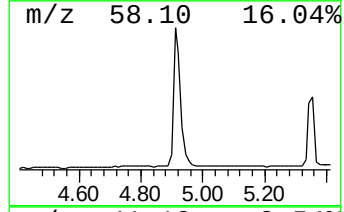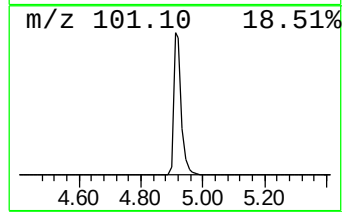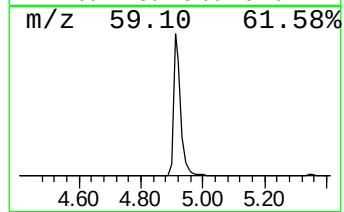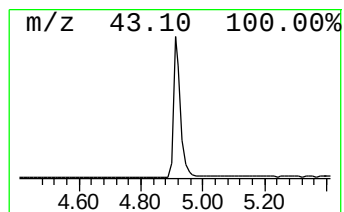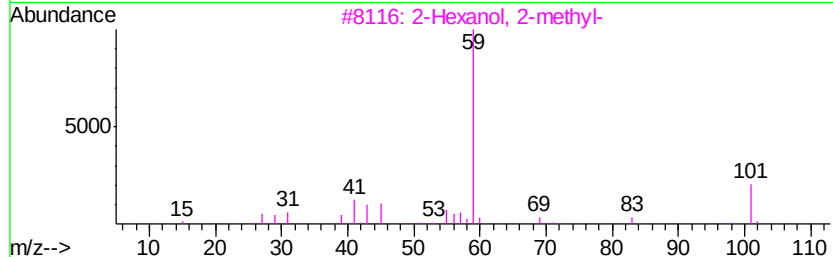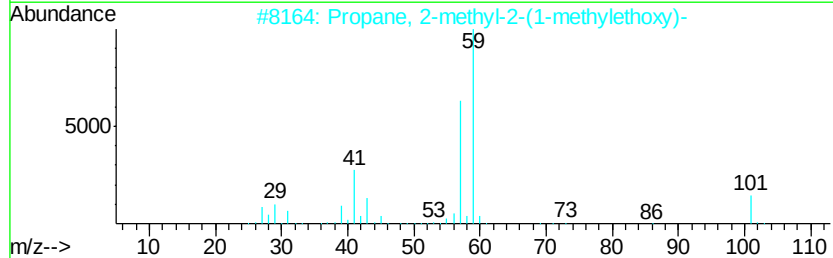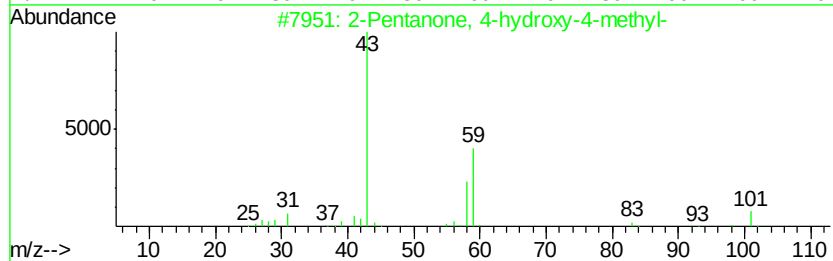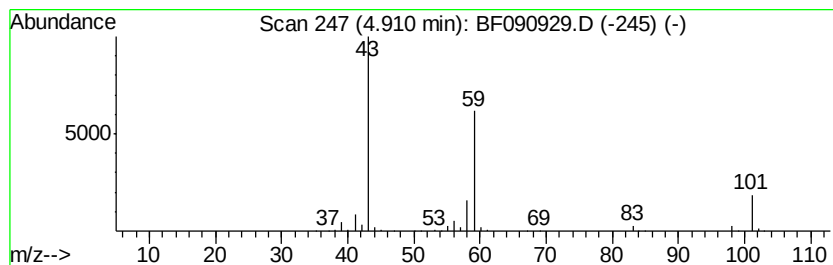

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103116\
Data File : BF090929.D
Acq On : 31 Oct 2016 15:44
Operator : UM/SJ
Sample : PB94407BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94407BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	104.55 ng	4597710	1,4-Dichlorobenzene-d4	6.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

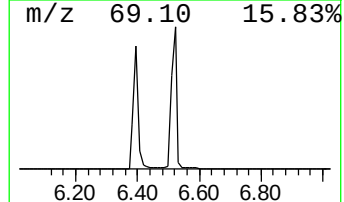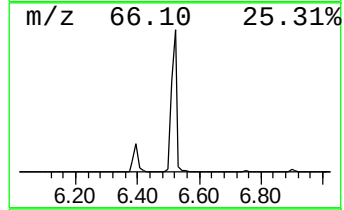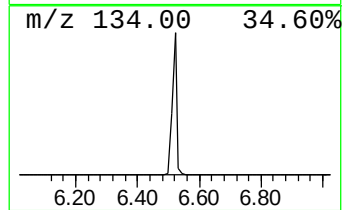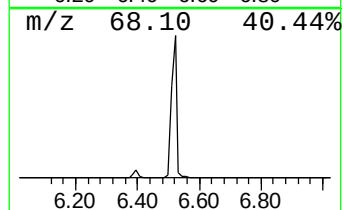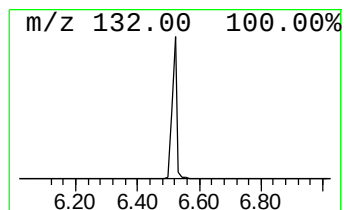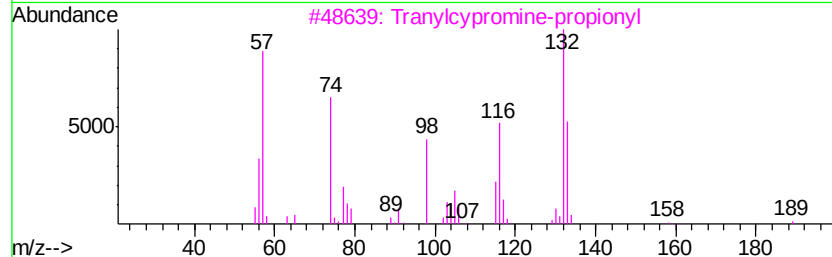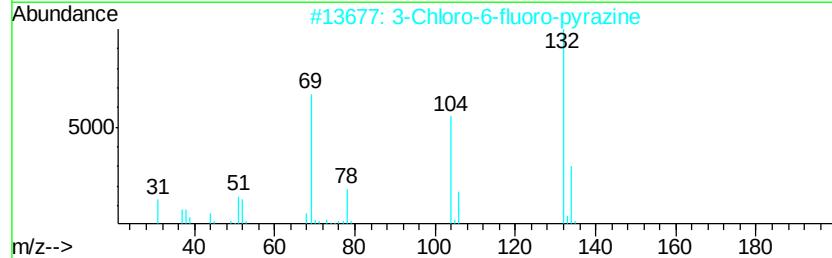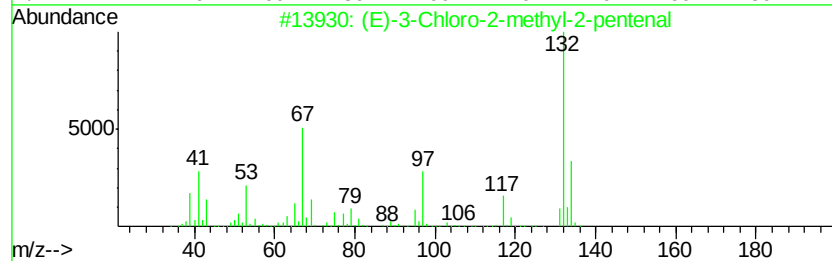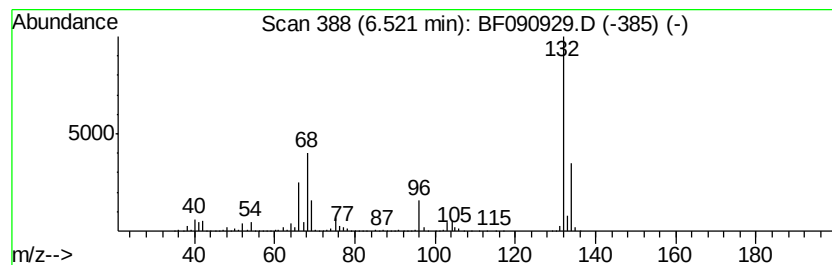

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103116\
Data File : BF090929.D
Acq On : 31 Oct 2016 15:44
Operator : UM/SJ
Sample : PB94407BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94407BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.91	20.1	ng	884041	1	6.75	879536	20.0
unknown6.52	6.52	104.6	ng	4597710	1	6.75	879536	20.0