


Data Path : Z:\HPCHEM1\BNA_F\Data\BF103116\
 Data File : BF090921.D
 Acq On : 31 Oct 2016 11:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 28 15:18:12 2016

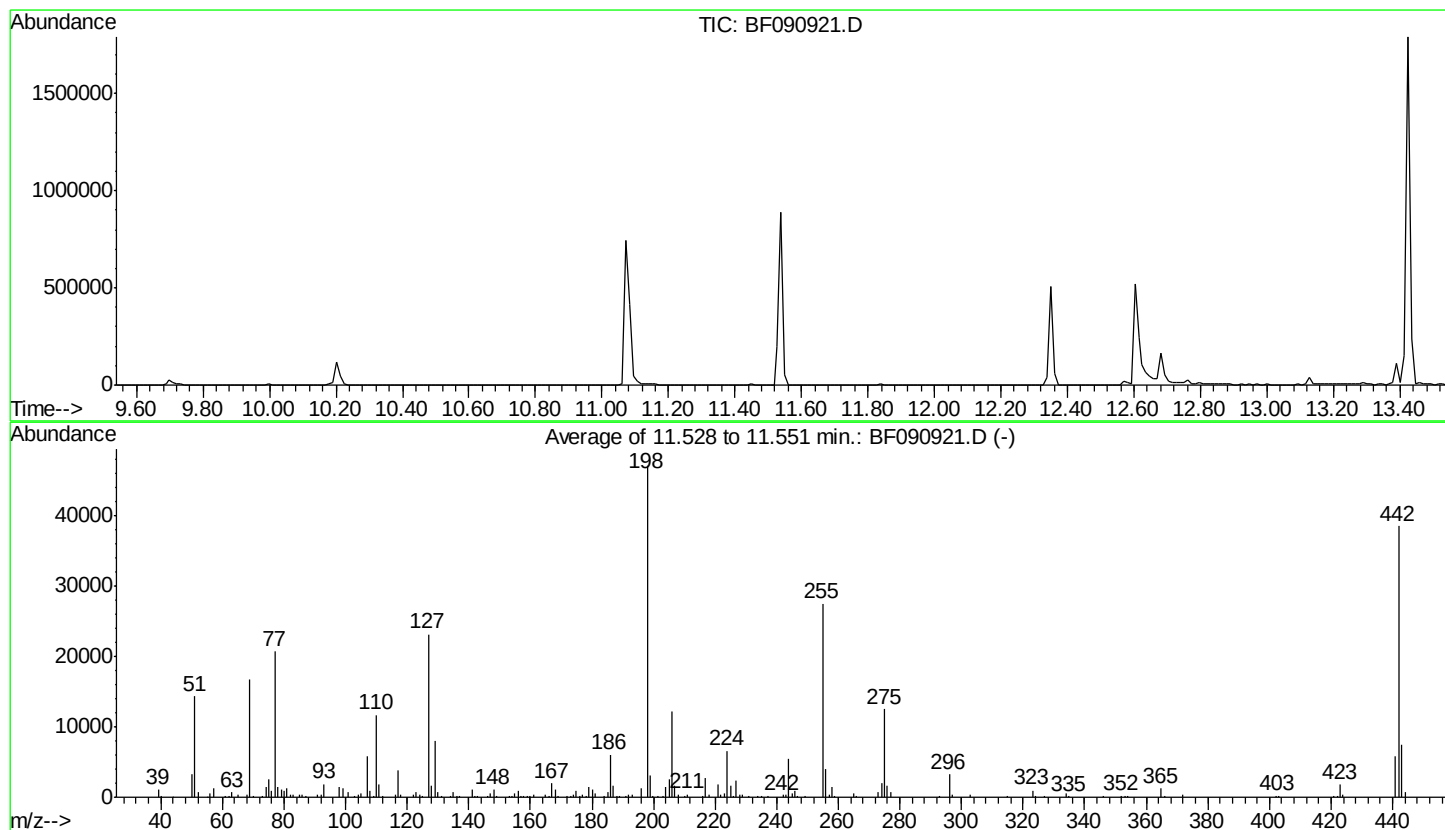

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	14306	PASS
68	69	0.00	2	1.7	290	PASS
69	198	0.00	100	35.6	16795	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	49.2	23196	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47125	PASS
199	198	5	9	6.4	3030	PASS
275	198	10	60	26.6	12521	PASS
365	198	1	100	2.5	1194	PASS
441	442	0.01	24	15.1	5806	PASS
442	198	50	100	81.7	38492	PASS
443	442	15	24	19.2	7378	PASS