

Data Path : Z:\HPCHEM1\BNA F\DATA\BF103117\
 Data File : BF100012.D
 Acq On : 31 Oct 2017 19:16
 Operator : SJ/JU
 Sample : I6178-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EPE-120-3(20-22)

Quant Time: Nov 01 05:22:32 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 31 16:51:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	81393	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	341725	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	157981	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	273765	20.00	ng	0.00
75) Chrysene-d12	13.97	240	162110	20.00	ng	-0.01
86) Perylene-d12	15.46	264	143579	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	533051	102.82	ng	0.00
7) Phenol-d6	6.43	99	636437	103.53	ng	0.00
23) Nitrobenzene-d5	7.36	82	357373	67.33	ng	0.00
41) 2,4,6-Tribromophenol	10.62	330	145834	101.29	ng	0.00
44) 2-Fluorobiphenyl	9.15	172	711268	69.46	ng	0.00
78) Terphenyl-d14	12.90	244	525018	70.78	ng	0.00
Target Compounds						
10) Phenol	6.45	94	47975	7.108	ng	96
49) Dimethylphthalate	9.54	163	215781	17.248	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF103117\
Data File : BF100012.D
Acq On : 31 Oct 2017 19:16
Operator : SJ/JU
Sample : I6178-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EPE-120-3(20-22)

Quant Time: Nov 01 05:22:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 16:51:57 2017
Response via : Initial Calibration

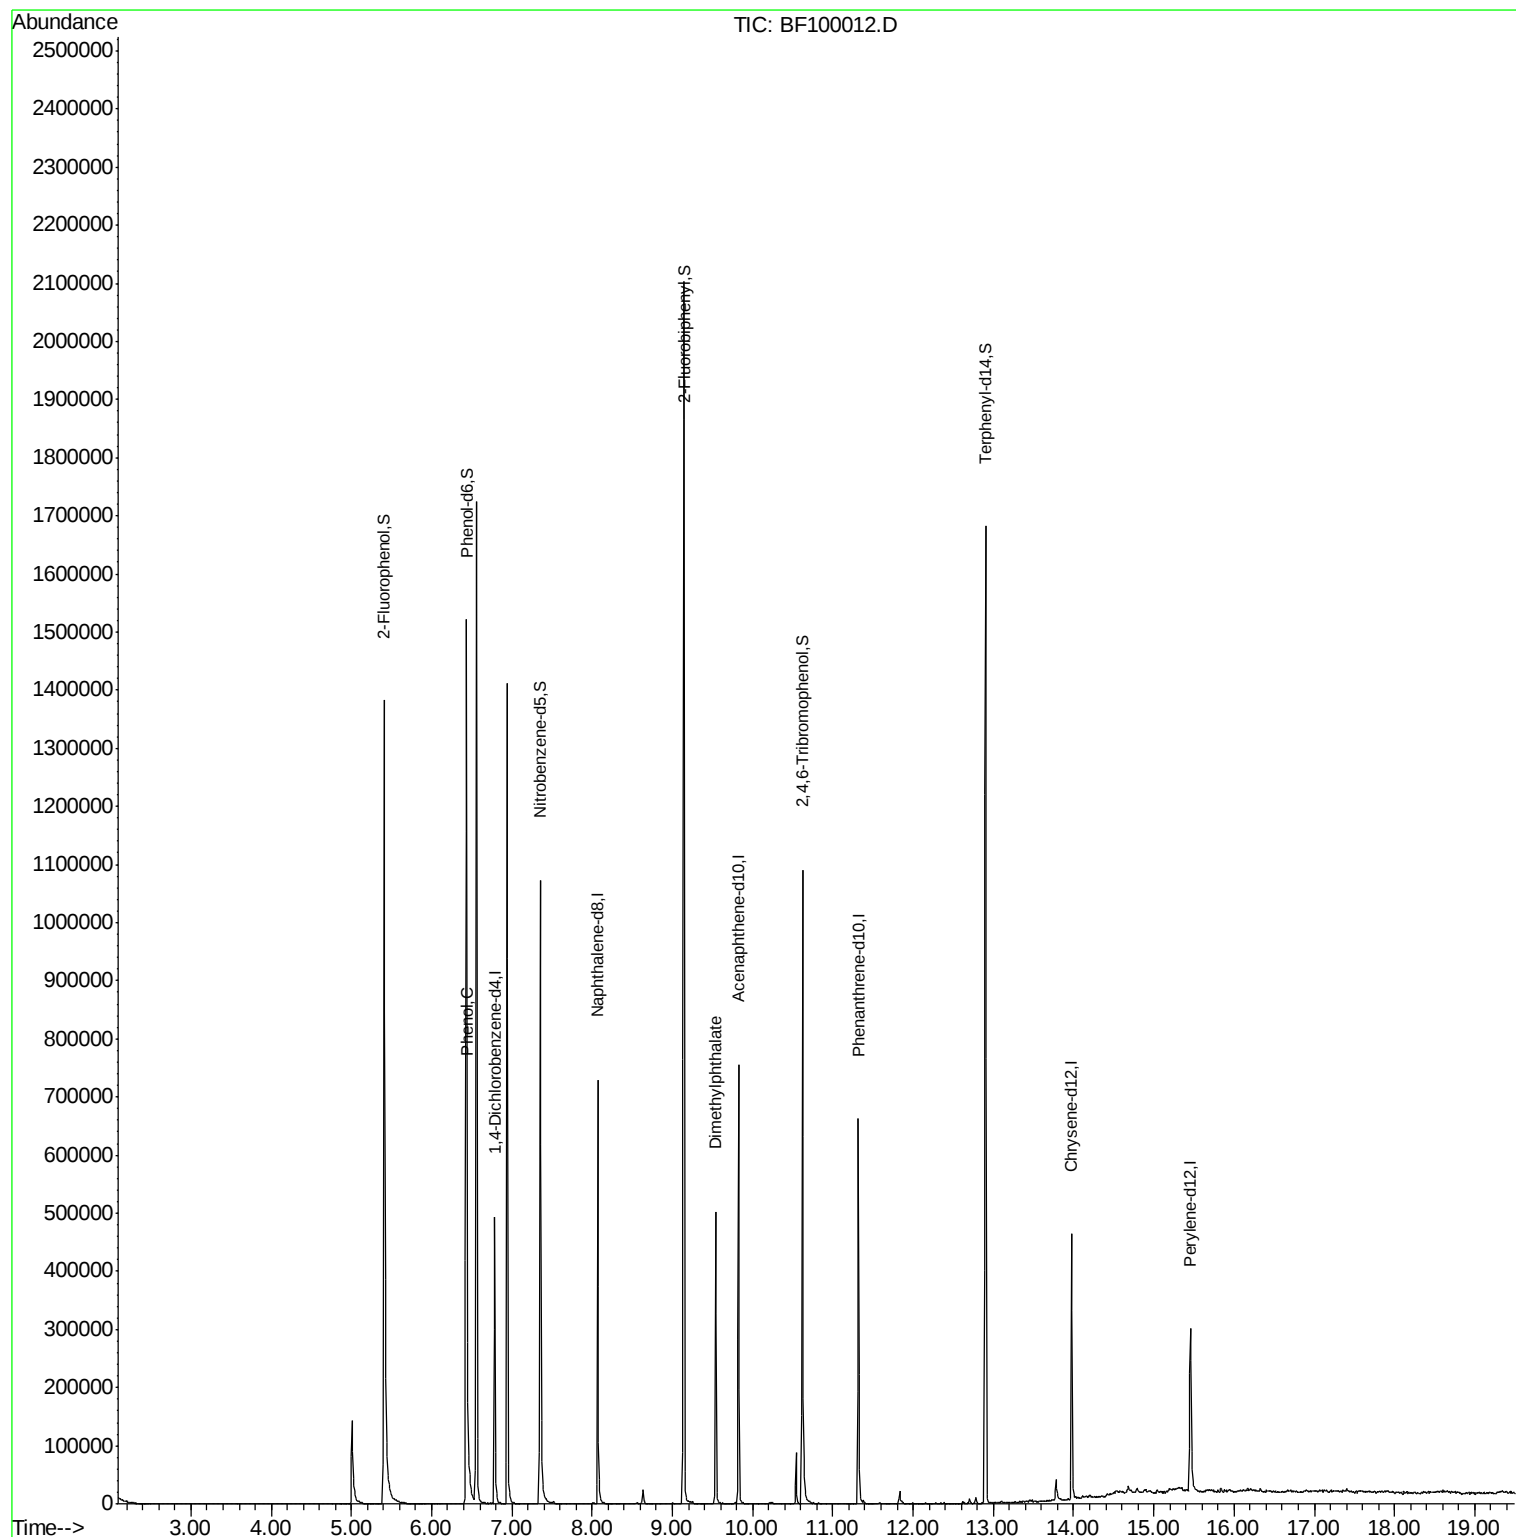




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. 0.00 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16

Instrument :
BNA_F
ClientSampleId :
EPE-120-3(20-22)

Tot Ion:152 Resp: 81393
Ion Ratio Lower Upper
152 100
150 153.5 124.6 186.8
115 58.3 50.1 75.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

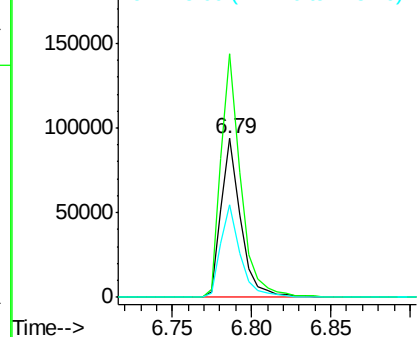



#5

2-Fluorophenol
Concen: 102.819 ng
RT: 5.41 min Scan# 565
Delta R.T. 0.01 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16

Tgt Ion:112 Resp: 533051
Ion Ratio Lower Upper
112 100
64 50.5 47.9 71.9
63 23.8 23.7 35.5

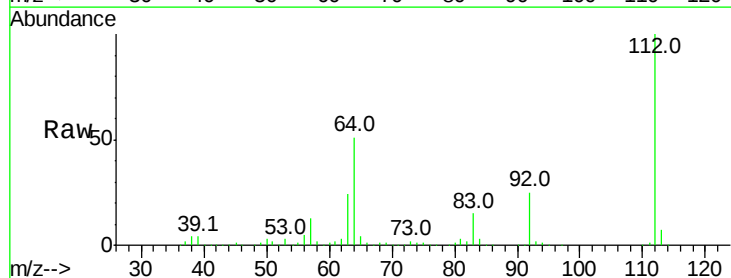

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

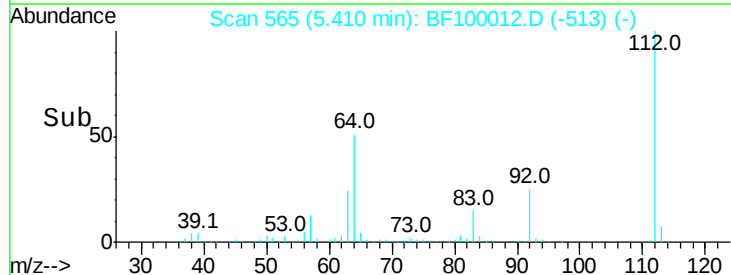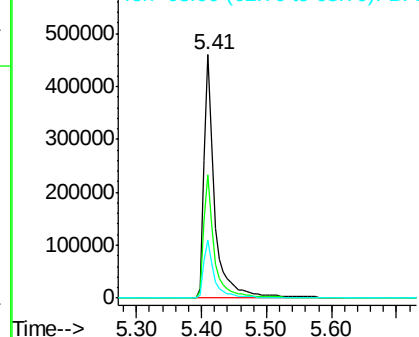



#7

Phenol-d6

Concen: 103.532 ng

RT: 6.43 min Scan# 739

Delta R.T. 0.00 min

Lab File: BF100012.D

Acq: 31 Oct 2017 19:16

Instrument :

BNA_F

ClientSampleId :

EPE-120-3(20-22)


Tot Ion: 99 Resp: 636437

Ion Ratio Lower Upper




99 100

42 13.1 14.5 21.7#

71 28.6 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

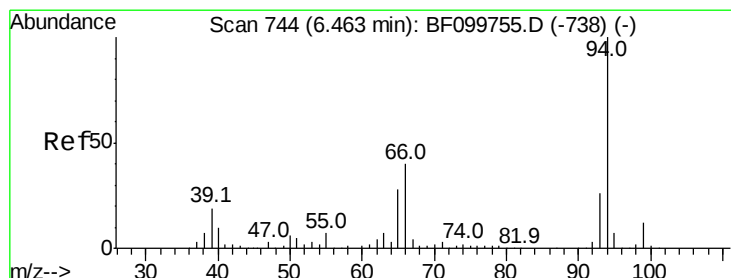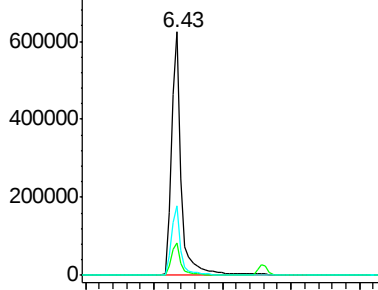

#10

Phenol

Concen: 7.108 ng

RT: 6.45 min Scan# 741

Delta R.T. 0.00 min

Lab File: BF100012.D

Acq: 31 Oct 2017 19:16


Tgt Ion: 94 Resp: 47975

Ion Ratio Lower Upper



94 100


65 25.2 7.9 47.9

66 38.0 16.2 56.2

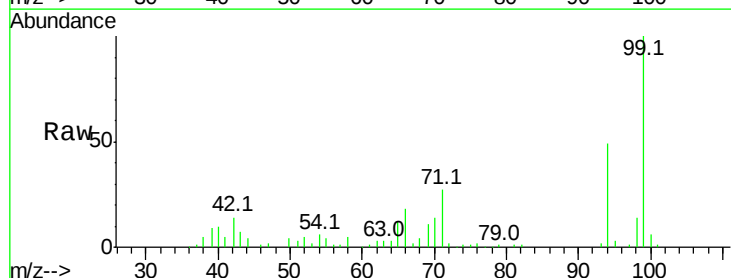

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

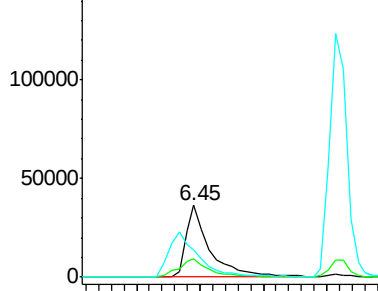


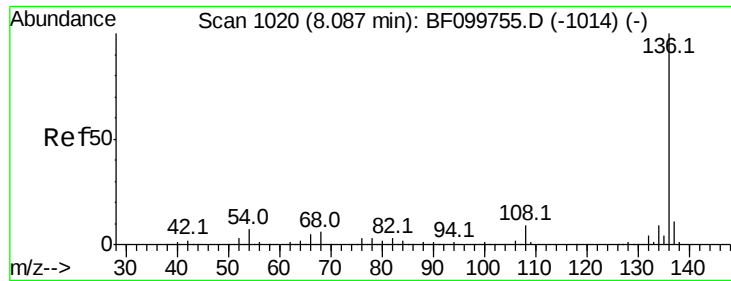




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.07 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16

Instrument :
BNA_F
ClientSampleId :
EPE-120-3(20-22)

Tot Ion:	136	Resp:	341725
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	6.2	6.6	9.8#
68	5.5	5.0	7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

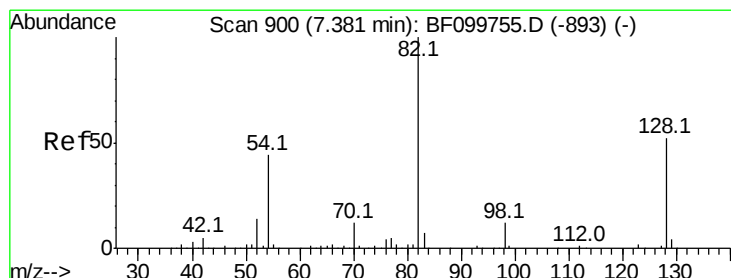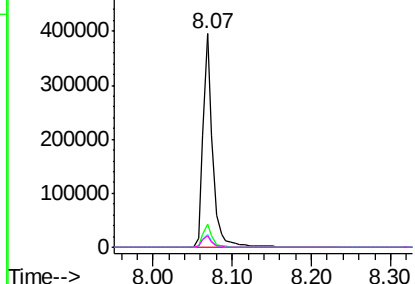



#23
Nitrobenzene-d5
Concen: 67.329 ng
RT: 7.36 min Scan# 896
Delta R.T. -0.01 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16

Tgt Ion:	82	Resp:	357373
Ion	Ratio	Lower	Upper
82	100		
128	49.6	36.1	54.1
54	45.3	41.4	62.2

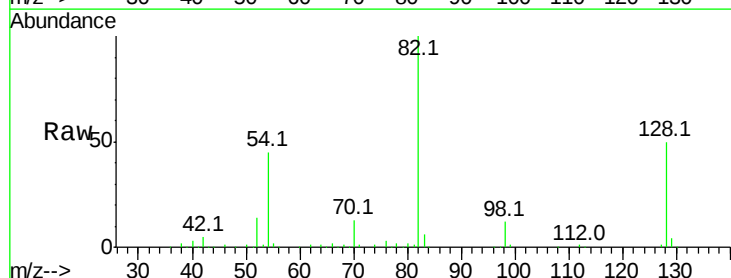

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1



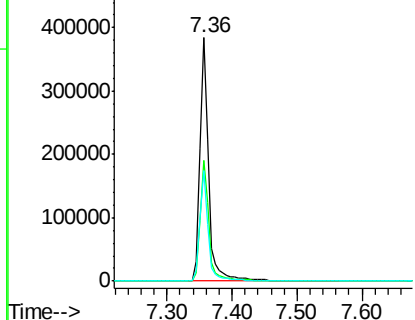





#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.82 min Scan# 1315
Delta R.T. -0.01 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16




Instrument :
BNA_F
ClientSampleId :
EPE-120-3(20-22)

Tot Ion:164 Resp: 157981
Ion Ratio Lower Upper
164 100
162 100.9 86.1 129.1
160 44.3 38.3 57.5

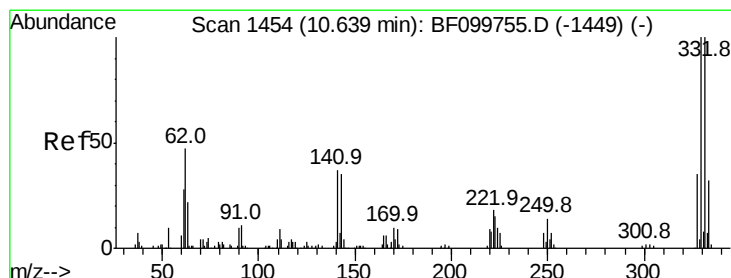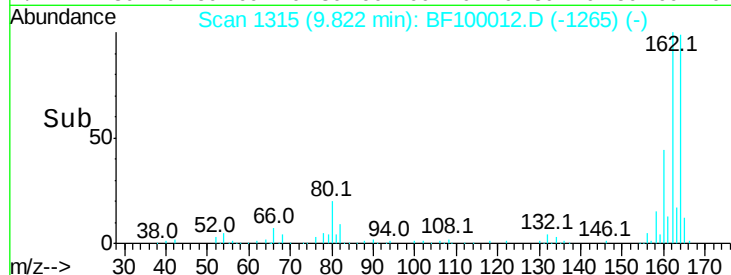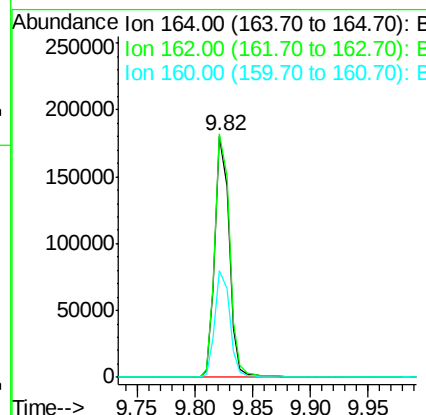

#41
2,4,6-Tribromophenol
Concen: 101.294 ng
RT: 10.62 min Scan# 1451
Delta R.T. -0.01 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16

Tgt Ion:330 Resp: 145834
Ion Ratio Lower Upper
330 100
332 97.9 77.0 115.6
141 33.9 29.9 44.9



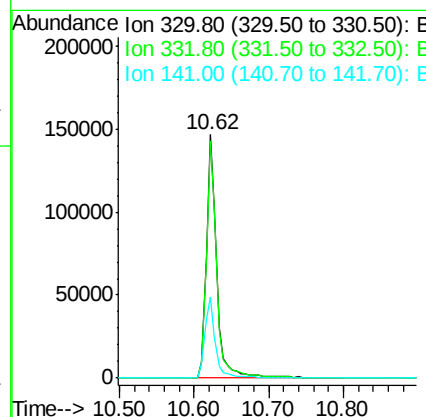
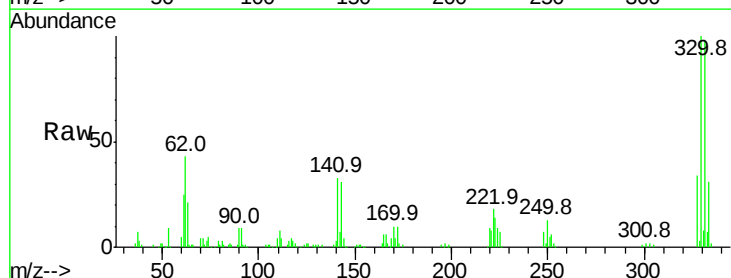




#44
2-Fluorobiphenyl
Concen: 69.462 ng
RT: 9.15 min Scan# 1200
Delta R.T. 0.00 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16




Instrument :
BNA_F
ClientSampleId :
EPE-120-3(20-22)


Tot Ion:172 Resp: 711268
Ion Ratio Lower Upper
172 100
171 35.4 29.7 44.5
170 23.6 19.6 29.4

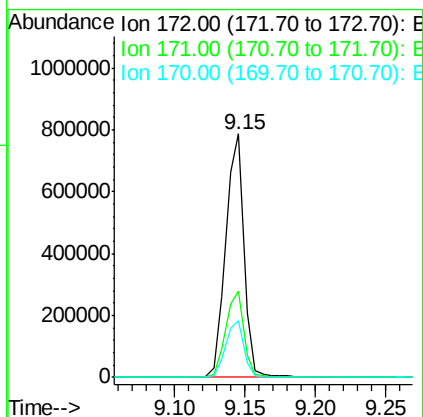

#49
Dimethylphthalate
Concen: 17.248 ng
RT: 9.54 min Scan# 1267
Delta R.T. -0.01 min
Lab File: BF100012.D
Acq: 31 Oct 2017 19:16

Tgt Ion:163 Resp: 215781
Ion Ratio Lower Upper
163 100
194 3.3 2.7 4.1
164 10.3 8.2 12.2

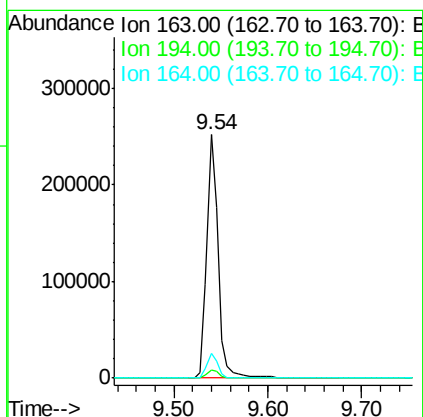







#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.32 min Scan# 1569
 Delta R.T. -0.01 min
 Lab File: BF100012.D
 Acq: 31 Oct 2017 19:16

Instrument :
 BNA_F
 ClientSampleId :
 EPE-120-3(20-22)

Tot Ion:188 Resp: 273765
 Ion Ratio Lower Upper
 188 100
 94 11.3 8.5 12.7
 80 11.6 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

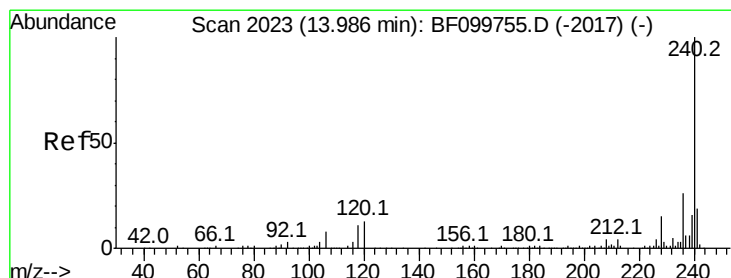
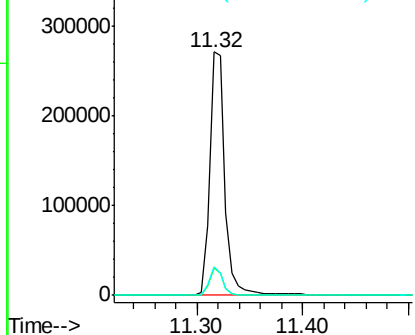



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.97 min Scan# 2021
 Delta R.T. -0.01 min
 Lab File: BF100012.D
 Acq: 31 Oct 2017 19:16

Tgt Ion:240 Resp: 162110
 Ion Ratio Lower Upper
 240 100
 120 14.3 9.5 14.3
 236 25.9 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

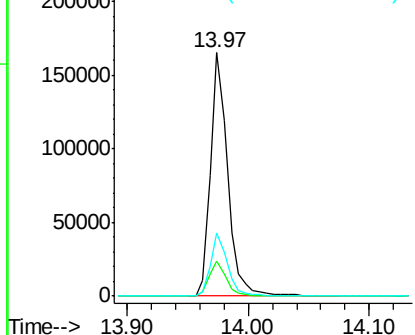

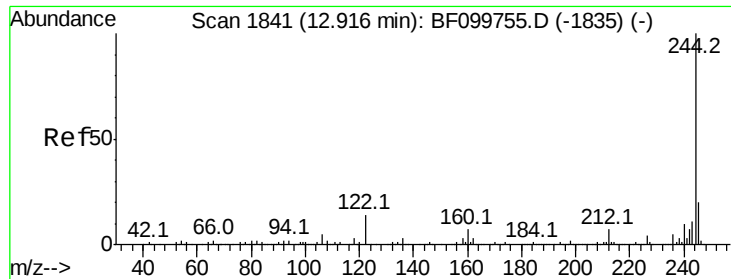

#78

Terphenyl-d14

Concen: 70.777 ng

RT: 12.90 min Scan# 1839

Delta R.T. 0.00 min

Lab File: BF100012.D

Acq: 31 Oct 2017 19:16

Instrument :

BNA_F

ClientSampleId :

EPE-120-3(20-22)


Tot Ion:244 Resp: 525018

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0




122 13.2 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

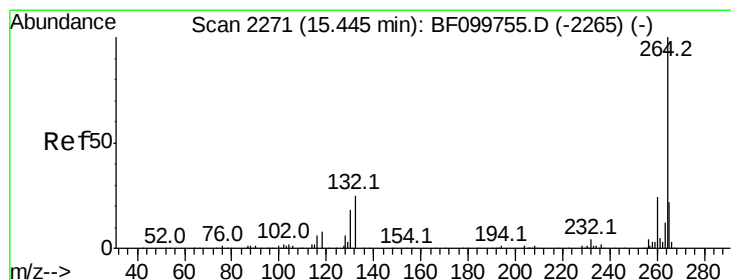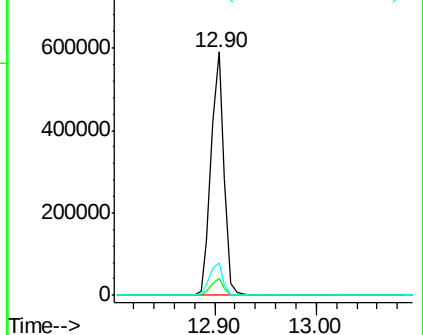

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2273

Delta R.T. -0.02 min

Lab File: BF100012.D

Acq: 31 Oct 2017 19:16


Tgt Ion:264 Resp: 143579

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 22.1 17.5 26.3

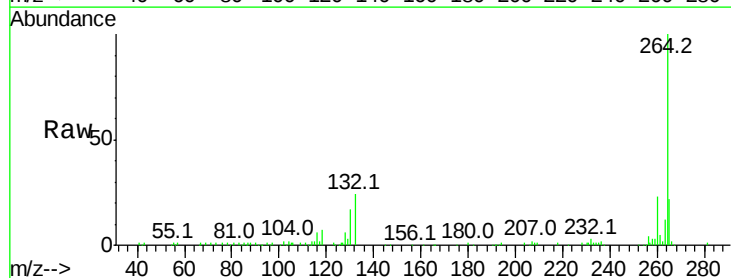

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

