

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
 Data File : BF100005.D
 Acq On : 31 Oct 2017 16:16
 Operator : SJ/JU
 Sample : PB103707BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB103707BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.004	493	496	522	rBV	196965	277943	11.92%	1.809%
2	5.416	563	566	591	rBV	732636	1040317	44.62%	6.769%
3	6.428	735	738	757	rBV	959532	1032220	44.27%	6.716%
4	6.557	757	760	769	rVB	1290690	1135627	48.70%	7.389%
5	6.786	796	799	812	rVB	478130	447835	19.21%	2.914%
6	6.939	821	825	843	rBV	1483188	1330538	57.06%	8.658%
7	7.357	892	896	911	rBV	1024779	961440	41.23%	6.256%
8	8.069	1013	1017	1042	rBV	718224	661276	28.36%	4.303%
9	9.139	1195	1199	1203	rBV	2115243	2075659	89.02%	13.506%
10	9.822	1311	1315	1327	rBV	887538	797171	34.19%	5.187%
11	10.622	1447	1451	1472	rBV	748224	823237	35.31%	5.357%
12	11.321	1566	1570	1579	rBV	873362	891287	38.22%	5.799%
13	12.904	1835	1839	1843	rBV	2196258	2331742	100.00%	15.172%
14	13.980	2018	2022	2036	rBV	887390	843960	36.19%	5.491%
15	15.439	2266	2270	2272	rBV2	21977	25784	1.11%	0.168%
16	15.474	2272	2276	2291	rVB	431229	630230	27.03%	4.101%
17	15.862	2338	2342	2350	rVB4	18872	28930	1.24%	0.188%
18	16.351	2420	2425	2431	rBV2	19715	33420	1.43%	0.217%


Sum of corrected areas: 15368616

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100005.D
Acq On : 31 Oct 2017 16:16
Operator : SJ/JU
Sample : PB103707BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103707BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

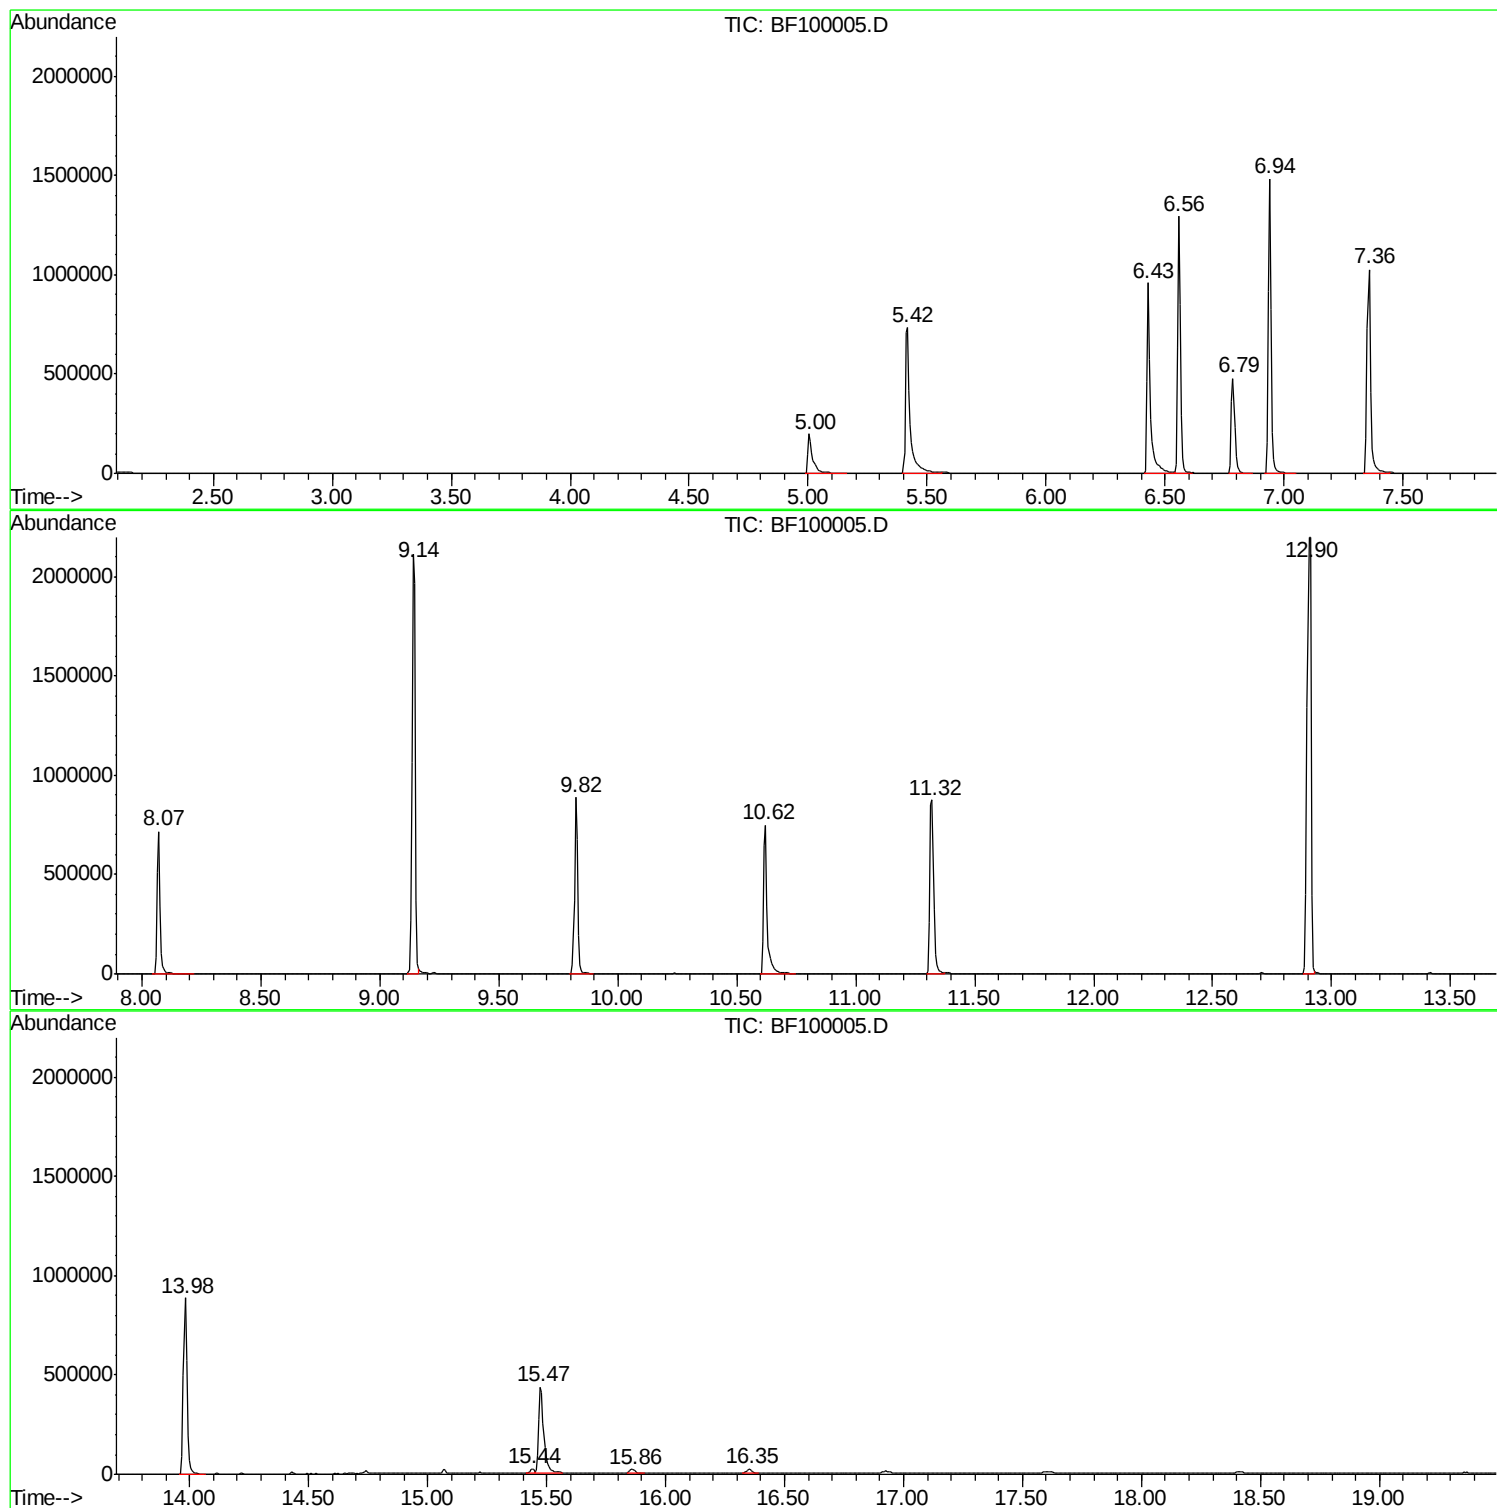

Data Path : Z:\HPCHEM1\BNA F\DATA\BF103117\
Data File : BF100005.D
Acq On : 31 Oct 2017 16:16
Operator : SJ/JU
Sample : PB103707BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103707BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.00	12.41 ng	277943	1,4-Dichlorobenzene-d4	6.79

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38
3			Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	35
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
5			3-Hexanol	102	C6H14O	000623-37-0	25

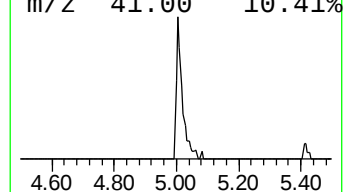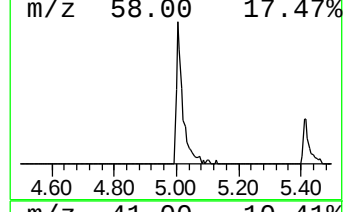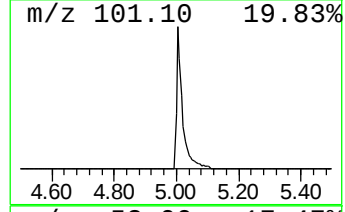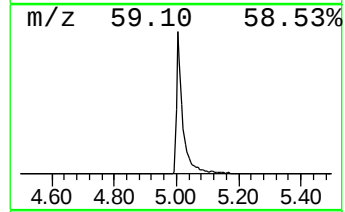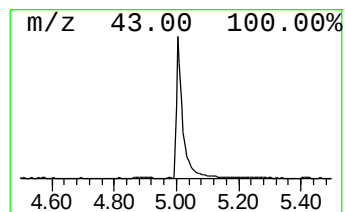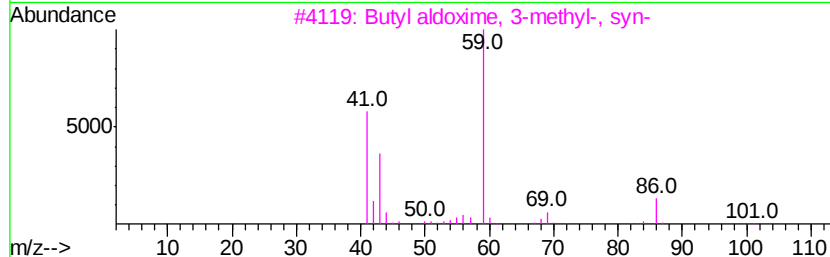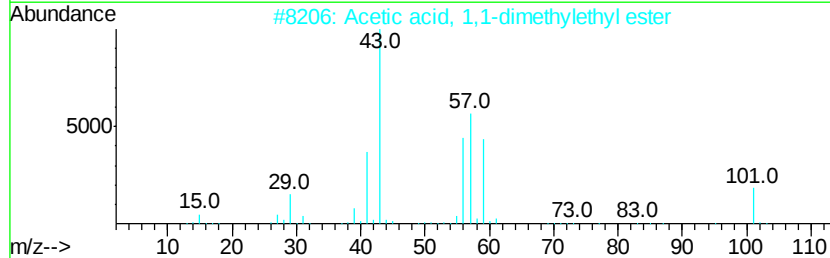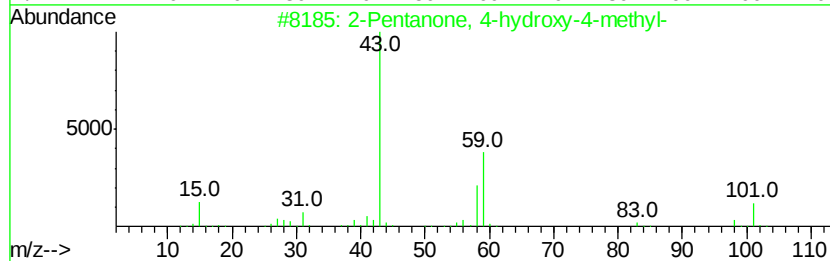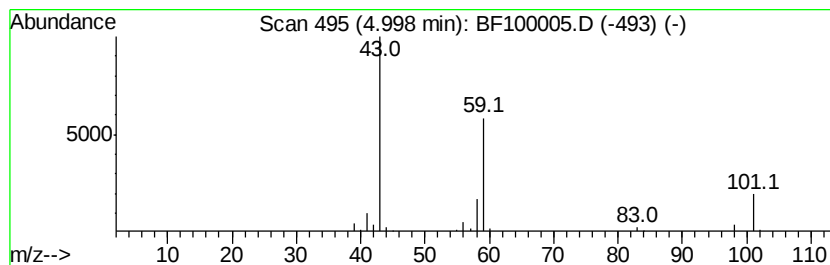

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100005.D
Acq On : 31 Oct 2017 16:16
Operator : SJ/JU
Sample : PB103707BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103707BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.56 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	50.72 ng	1135630	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

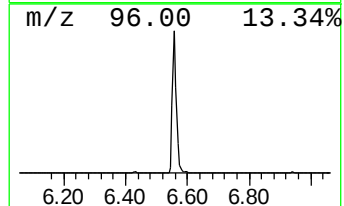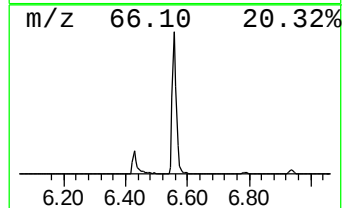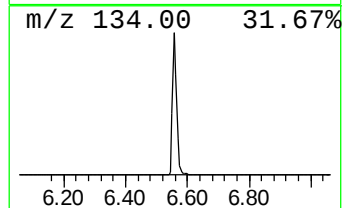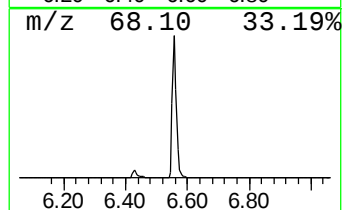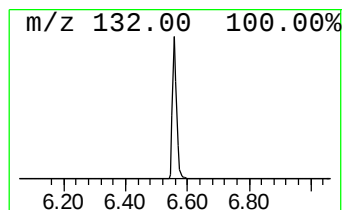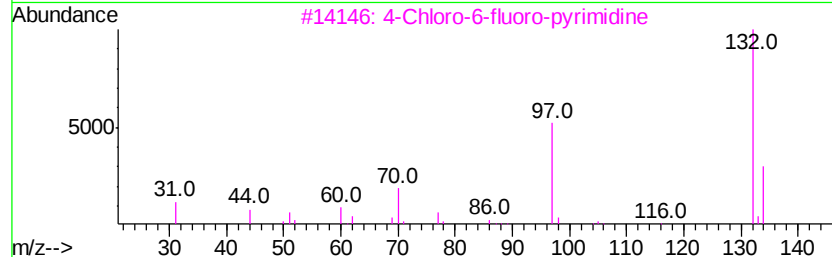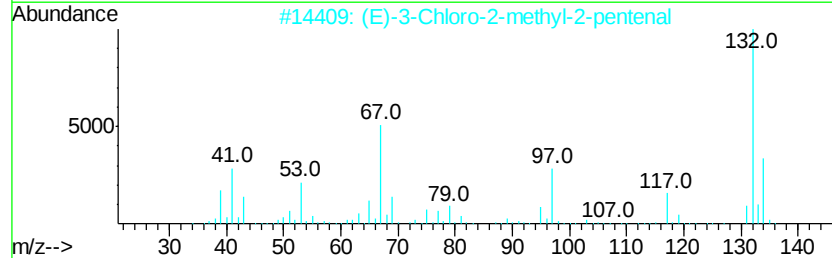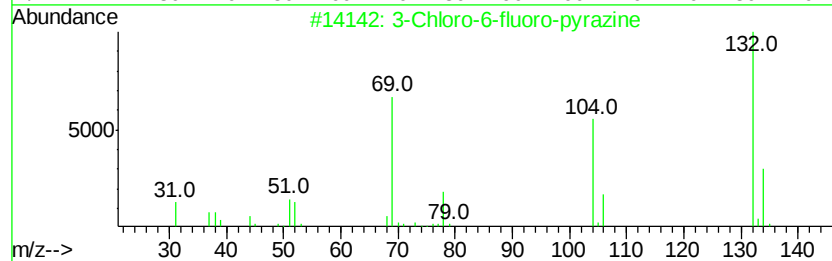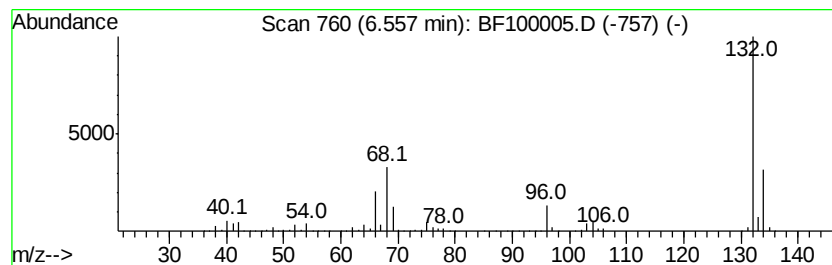

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100005.D
Acq On : 31 Oct 2017 16:16
Operator : SJ/JU
Sample : PB103707BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103707BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.00	12.4	ng	277943	1	6.79	447835	20.0
unknown6.56	6.56	50.7	ng	1135630	1	6.79	447835	20.0