

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
 Data File : BF100018.D
 Acq On : 31 Oct 2017 21:51
 Operator : SJ/JU
 Sample : I6056-03 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SED-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.310	31	38	47	rVB2	22002	38223	5.43%	0.516%
2	4.998	492	495	503	rBV	16222	28633	4.06%	0.387%
3	5.416	563	566	586	rBV	128318	238729	33.88%	3.224%
4	6.439	737	740	758	rBV	153095	277938	39.45%	3.753%
5	6.563	758	761	767	rBV	283582	301078	42.73%	4.066%
6	6.786	796	799	810	rBV	551114	491181	69.72%	6.633%
7	6.939	822	825	843	rBB	250232	252901	35.90%	3.415%
8	7.363	893	897	911	rBV	106171	159630	22.66%	2.156%
9	8.069	1014	1017	1032	rBV	773163	663902	94.23%	8.965%
10	9.139	1196	1199	1209	rBV	449747	389765	55.32%	5.263%
11	9.545	1265	1268	1276	rBV	35890	30321	4.30%	0.409%
12	9.827	1312	1316	1331	rVB	756831	704551	100.00%	9.514%
13	10.545	1434	1438	1441	rBV	16585	16374	2.32%	0.221%
14	10.627	1448	1452	1464	rVB	118940	140835	19.99%	1.902%
15	11.168	1537	1544	1546	rBV4	6542	10600	1.50%	0.143%
16	11.321	1566	1570	1572	rBV	705328	645196	91.58%	8.712%
17	11.345	1572	1574	1579	rVV	115035	116041	16.47%	1.567%
18	11.404	1582	1584	1587	rVB	13389	10476	1.49%	0.141%
19	11.580	1609	1614	1618	rBV2	5884	10750	1.53%	0.145%
20	11.827	1653	1656	1659	rBV2	18297	25343	3.60%	0.342%
21	11.857	1659	1661	1666	rVB2	23072	21726	3.08%	0.293%
22	11.939	1672	1675	1678	rBV	20710	22993	3.26%	0.310%
23	11.963	1678	1679	1683	rVB	12833	7415	1.05%	0.100%
24	12.121	1701	1706	1709	rBV3	11238	16037	2.28%	0.217%
25	12.180	1714	1716	1720	rVB4	9399	11444	1.62%	0.155%
26	12.380	1747	1750	1753	rBV5	10015	13323	1.89%	0.180%
27	12.545	1775	1778	1781	rBV	153542	148732	21.11%	2.008%
28	12.657	1795	1797	1800	rVB2	11418	11287	1.60%	0.152%
29	12.774	1811	1817	1823	rBV	139047	153445	21.78%	2.072%
30	12.821	1823	1825	1829	rVB5	10559	14781	2.10%	0.200%
31	12.904	1836	1839	1842	rVB	362390	305474	43.36%	4.125%
32	13.104	1870	1873	1878	rVB5	22177	38062	5.40%	0.514%
33	13.339	1910	1913	1915	rBV2	14438	12162	1.73%	0.164%
34	13.792	1986	1990	1996	rVB2	87012	103859	14.74%	1.402%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100018.D
Acq On : 31 Oct 2017 21:51
Operator : SJ/JU
Sample : I6056-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SED-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.980	2018	2022	2026	rBV	501438	524510	74.45%	7.083%
36	14.009	2026	2027	2030	rVB	62332	41580	5.90%	0.561%
37	14.439	2095	2100	2108	rBV6	66512	170094	24.14%	2.297%
38	14.886	2173	2176	2178	rBV3	47668	49645	7.05%	0.670%
39	15.068	2201	2207	2210	rBV2	105459	199881	28.37%	2.699%
40	15.356	2253	2256	2263	rVB	40145	59463	8.44%	0.803%
41	15.421	2264	2267	2272	rVV2	56454	89832	12.75%	1.213%
42	15.474	2272	2276	2289	rVB	354952	502032	71.26%	6.779%
43	15.639	2300	2304	2309	rBV2	66999	87740	12.45%	1.185%
44	15.862	2339	2342	2347	rVB	48624	70331	9.98%	0.950%
45	16.645	2470	2475	2483	rVB2	62482	118267	16.79%	1.597%
46	17.439	2608	2610	2619	rVB3	28841	58998	8.37%	0.797%


Sum of corrected areas: 7405580

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100018.D
Acq On : 31 Oct 2017 21:51
Operator : SJ/JU
Sample : I6056-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SED-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

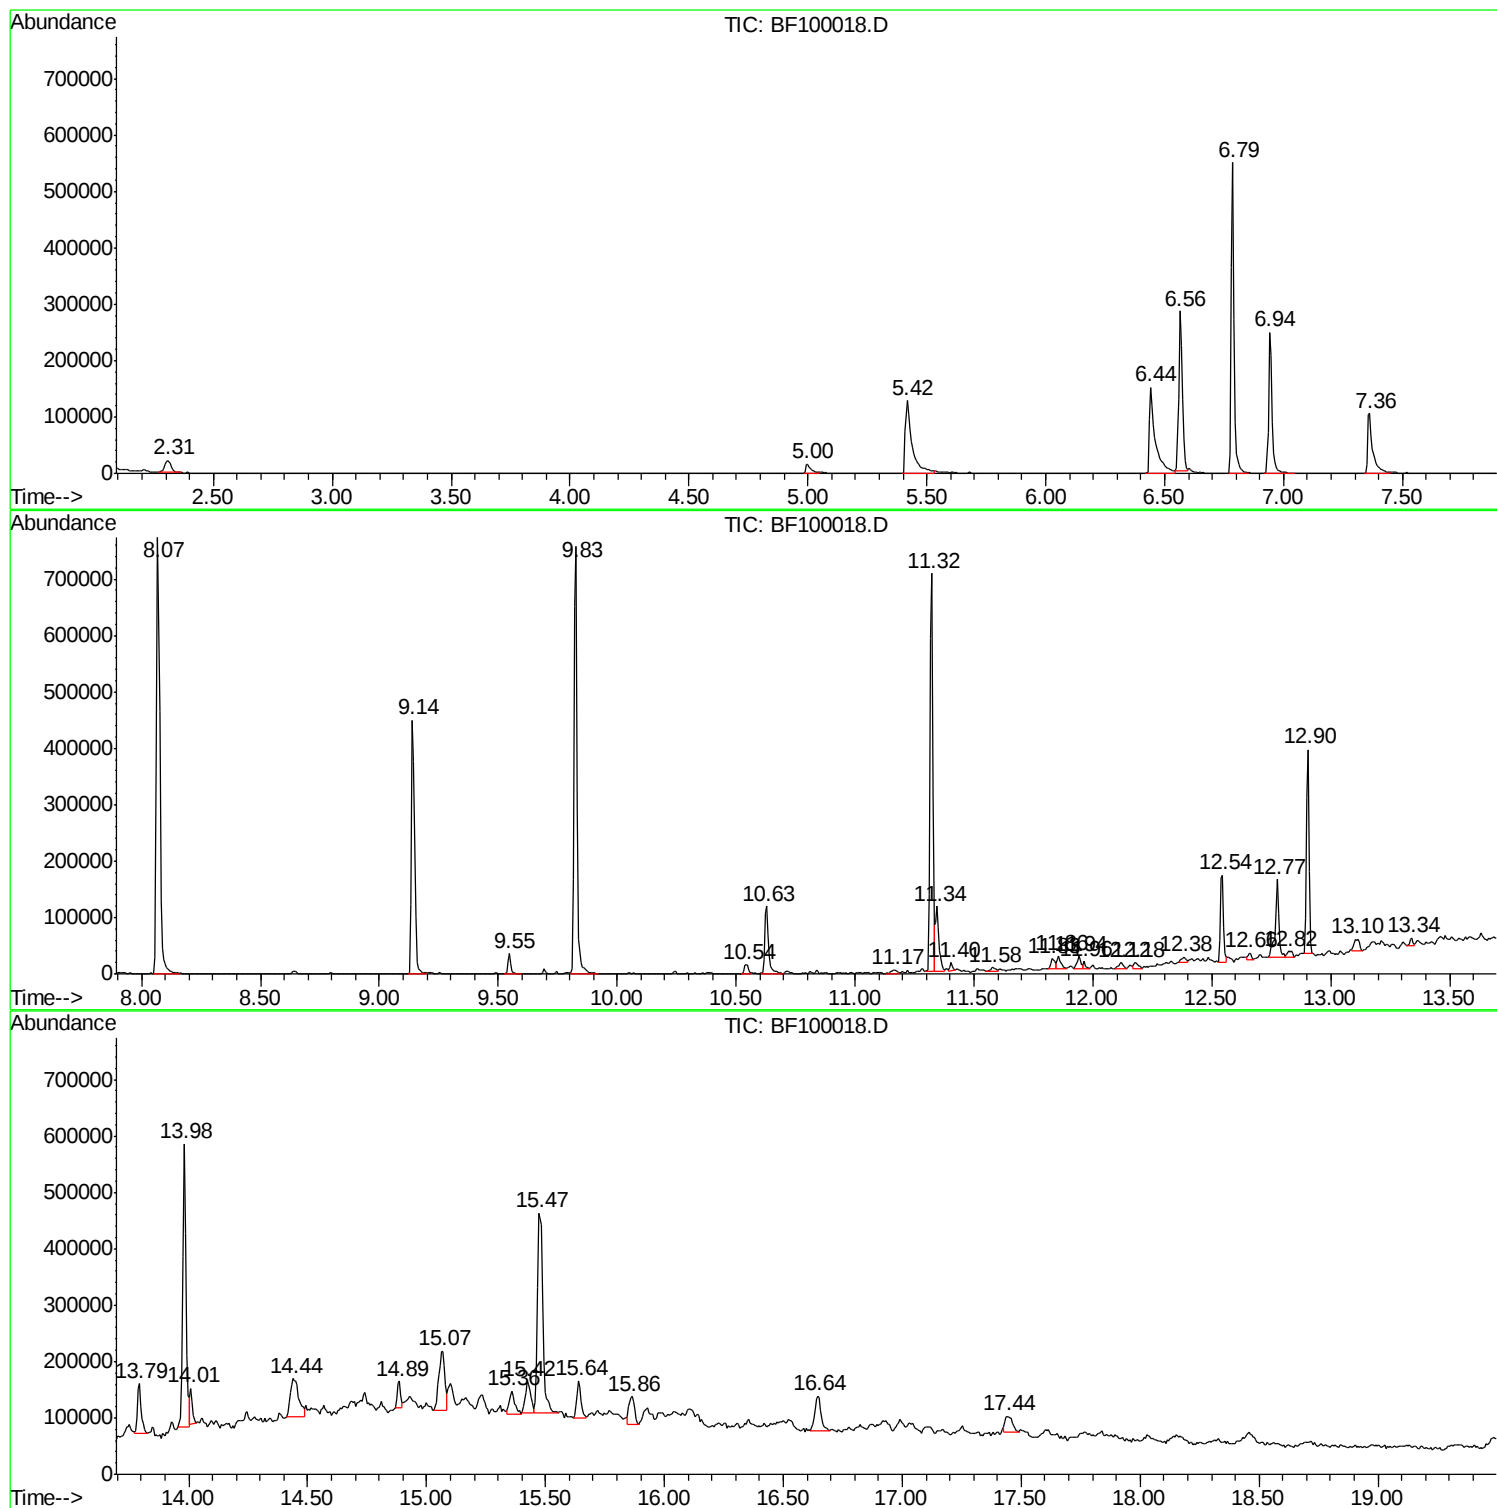

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100018.D
Acq On : 31 Oct 2017 21:51
Operator : SJ/JU
Sample : I6056-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SED-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100018.D
Acq On : 31 Oct 2017 21:51
Operator : SJ/JU
Sample : I6056-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SED-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc