

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
 Data File : BF100019.D
 Acq On : 31 Oct 2017 22:16
 Operator : SJ/JU
 Sample : I6056-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	43	50	63	rVB	51711	95884	3.81%	0.615%
2	4.998	492	495	515	rBV	65485	105855	4.21%	0.678%
3	5.410	562	565	598	rBV	667455	907081	36.03%	5.814%
4	6.433	736	739	757	rBV	428316	627455	24.93%	4.022%
5	6.563	757	761	775	rVB	1542673	1595497	63.38%	10.226%
6	6.786	796	799	809	rBV	550162	474353	18.84%	3.040%
7	6.939	822	825	845	rBV	1766246	1750614	69.54%	11.220%
8	7.363	893	897	918	rBV	1206890	1274870	50.64%	8.171%
9	8.069	1014	1017	1032	rBV	776196	651963	25.90%	4.179%
10	9.145	1196	1200	1203	rBV	2808690	2517330	100.00%	16.134%
11	9.539	1264	1267	1278	rVB	83959	77306	3.07%	0.495%
12	9.827	1312	1316	1326	rBV	744923	709227	28.17%	4.546%
13	10.539	1433	1437	1444	rBV	26812	27105	1.08%	0.174%
14	10.621	1448	1451	1465	rBV	1086274	1061425	42.16%	6.803%
15	11.321	1566	1570	1578	rBV	775797	688047	27.33%	4.410%
16	12.909	1835	1840	1843	rBV	2056908	1984882	78.85%	12.722%
17	13.980	2018	2022	2028	rBV	463926	458671	18.22%	2.940%
18	15.468	2271	2275	2283	rVB	350193	447706	17.78%	2.869%
19	17.027	2534	2540	2554	rVB10	37556	102812	4.08%	0.659%
20	17.409	2600	2605	2615	rVB9	15575	44316	1.76%	0.284%


Sum of corrected areas: 15602399

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100019.D
Acq On : 31 Oct 2017 22:16
Operator : SJ/JU
Sample : I6056-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

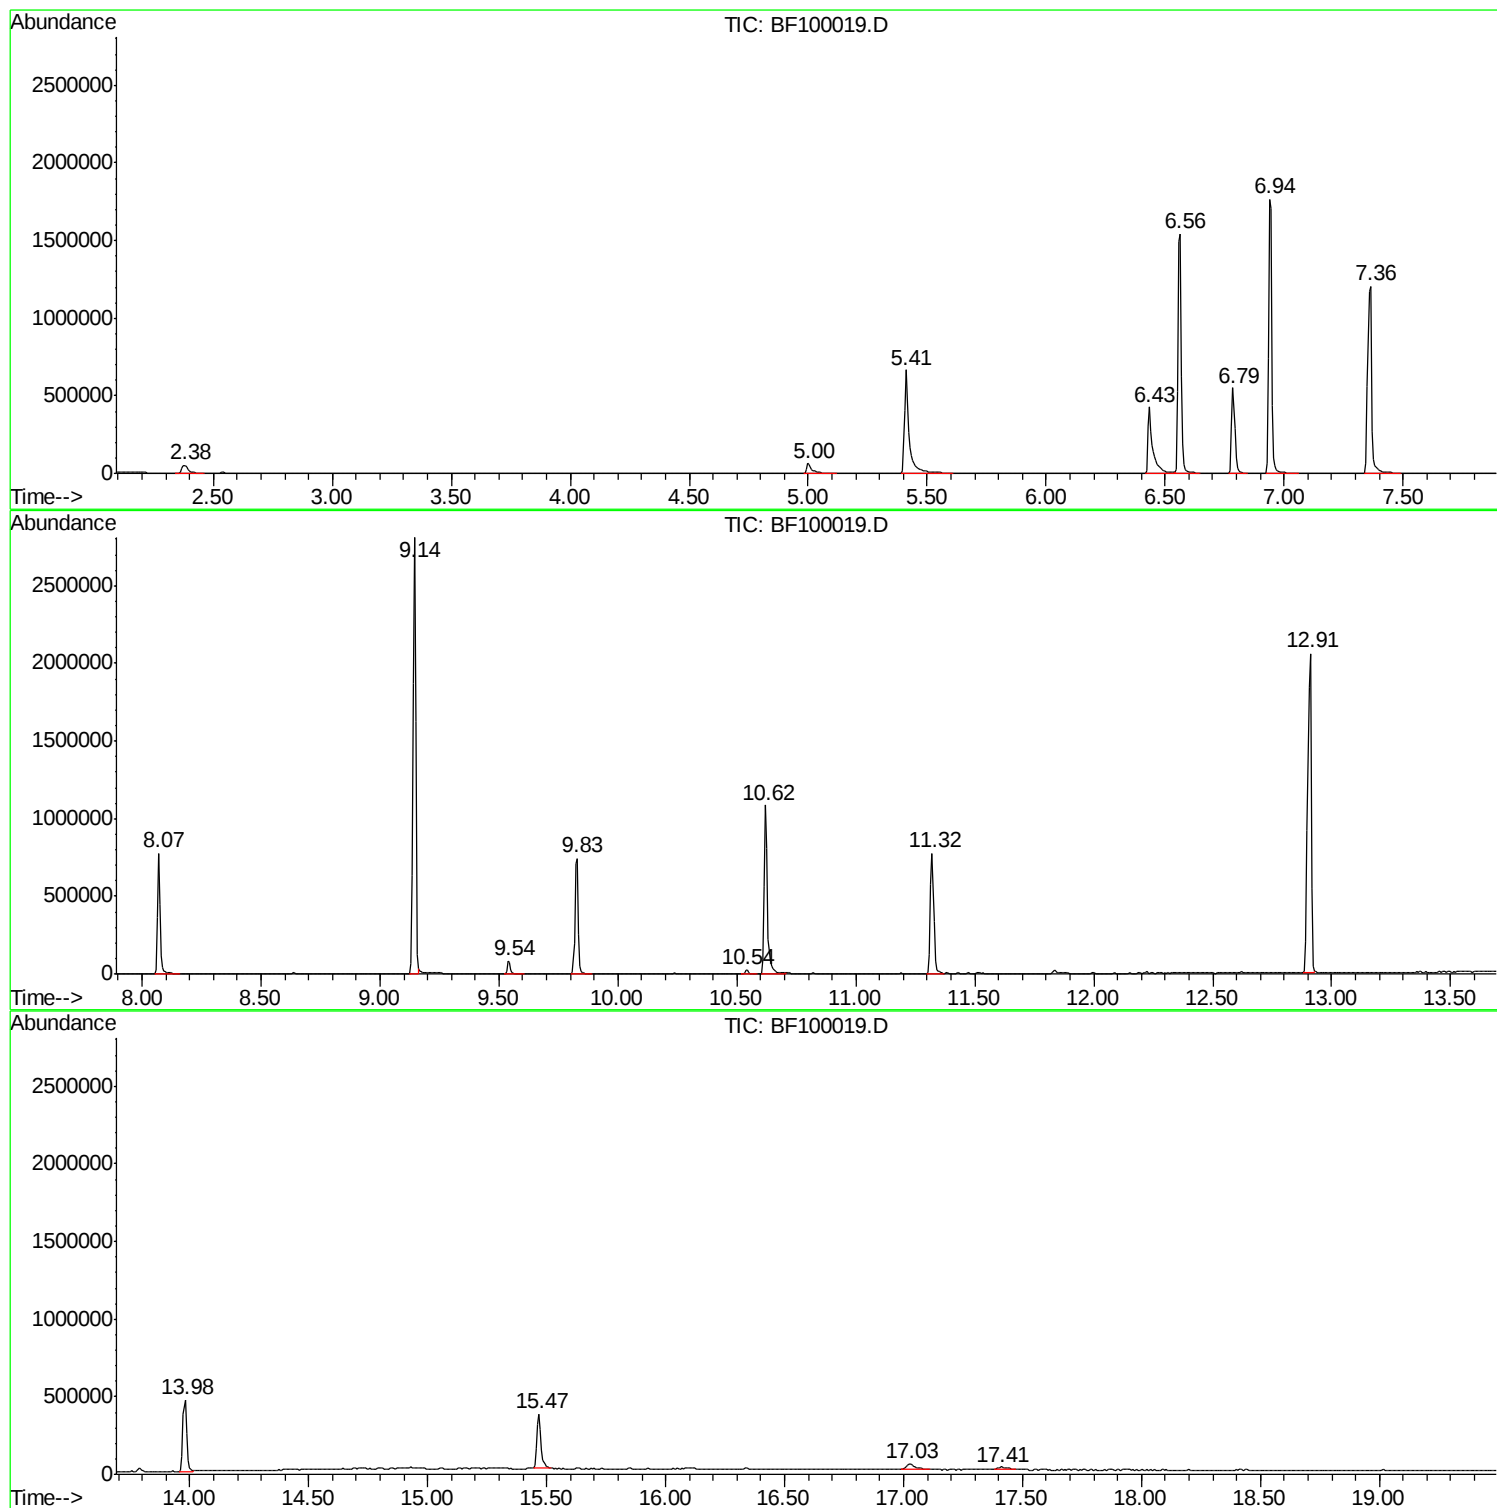

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100019.D
Acq On : 31 Oct 2017 22:16
Operator : SJ/JU
Sample : I6056-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
Data File : BF100019.D
Acq On : 31 Oct 2017 22:16
Operator : SJ/JU
Sample : I6056-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc