


Data Path : Z:\HPCHEM1\BNA F\DATA\BF103117\
 Data File : BF099998.D
 Acq On : 31 Oct 2017 13:09
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 31 16:51:57 2017

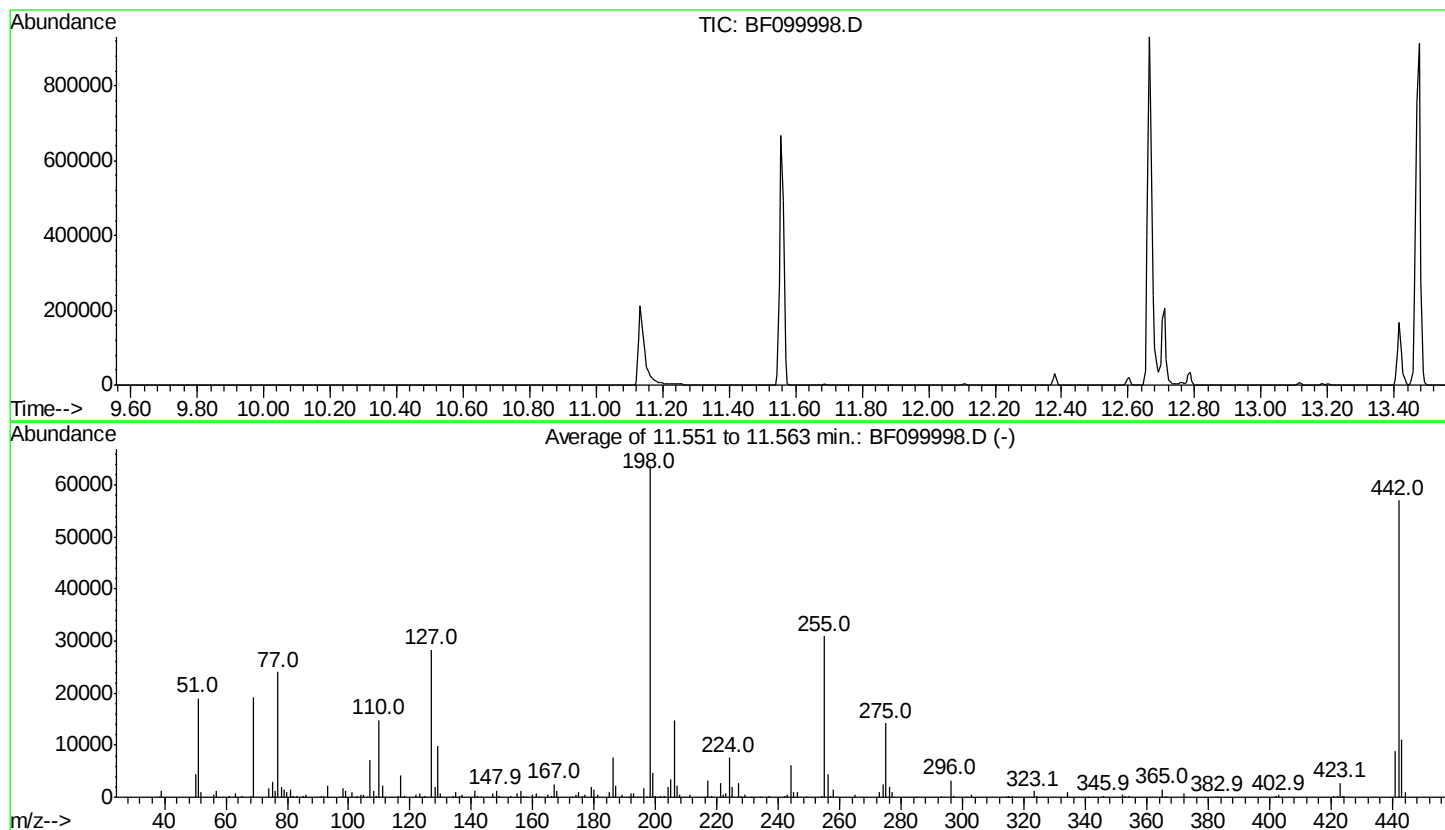

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	18965	PASS
68	69	0.00	2	1.4	272	PASS
69	198	0.00	100	30.0	19117	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	28349	PASS
197	198	0.00	2	0.2	115	PASS
198	198	100	100	100.0	63754	PASS
199	198	5	9	7.2	4579	PASS
275	198	10	60	22.3	14232	PASS
365	198	1	100	2.5	1599	PASS
441	443	0.01	100	79.6	8783	PASS
442	198	50	100	89.5	57079	PASS
443	442	15	24	19.3	11040	PASS