


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF103117\
 Data File : BF100024.D
 Acq On : 1 Nov 2017 3:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 31 16:51:57 2017

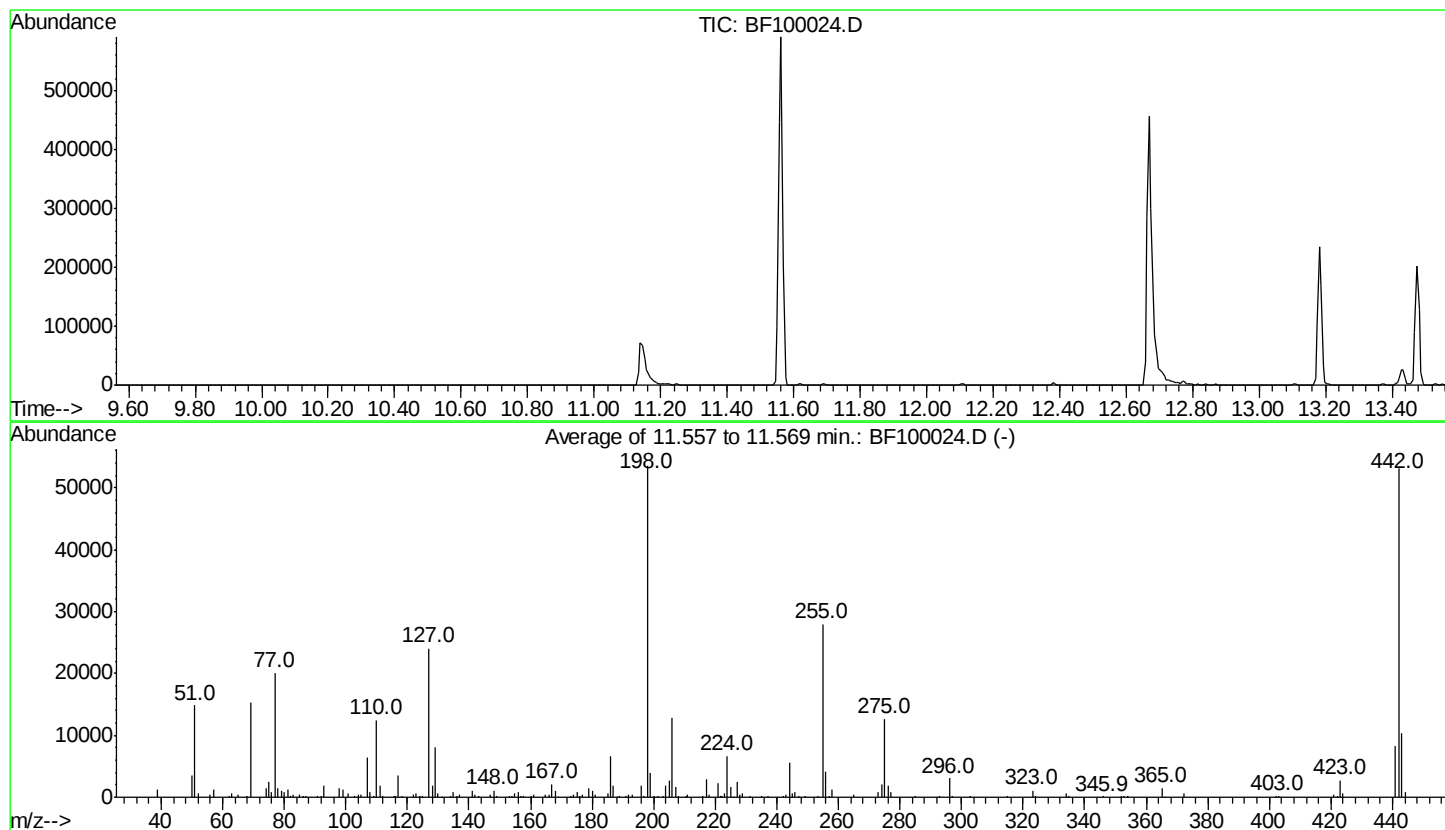

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	14807	PASS
68	69	0.00	2	0.9	138	PASS
69	198	0.00	100	28.6	15312	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	24077	PASS
197	198	0.00	2	0.4	232	PASS
198	198	100	100	100.0	53597	PASS
199	198	5	9	7.2	3841	PASS
275	198	10	60	23.7	12700	PASS
365	198	1	100	2.7	1472	PASS
441	443	0.01	100	80.6	8312	PASS
442	198	50	100	99.4	53282	PASS
443	442	15	24	19.3	10308	PASS