


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103122\
 Data File : BF130871.D
 Acq On : 31 Oct 2022 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 02 08:18:35 2022

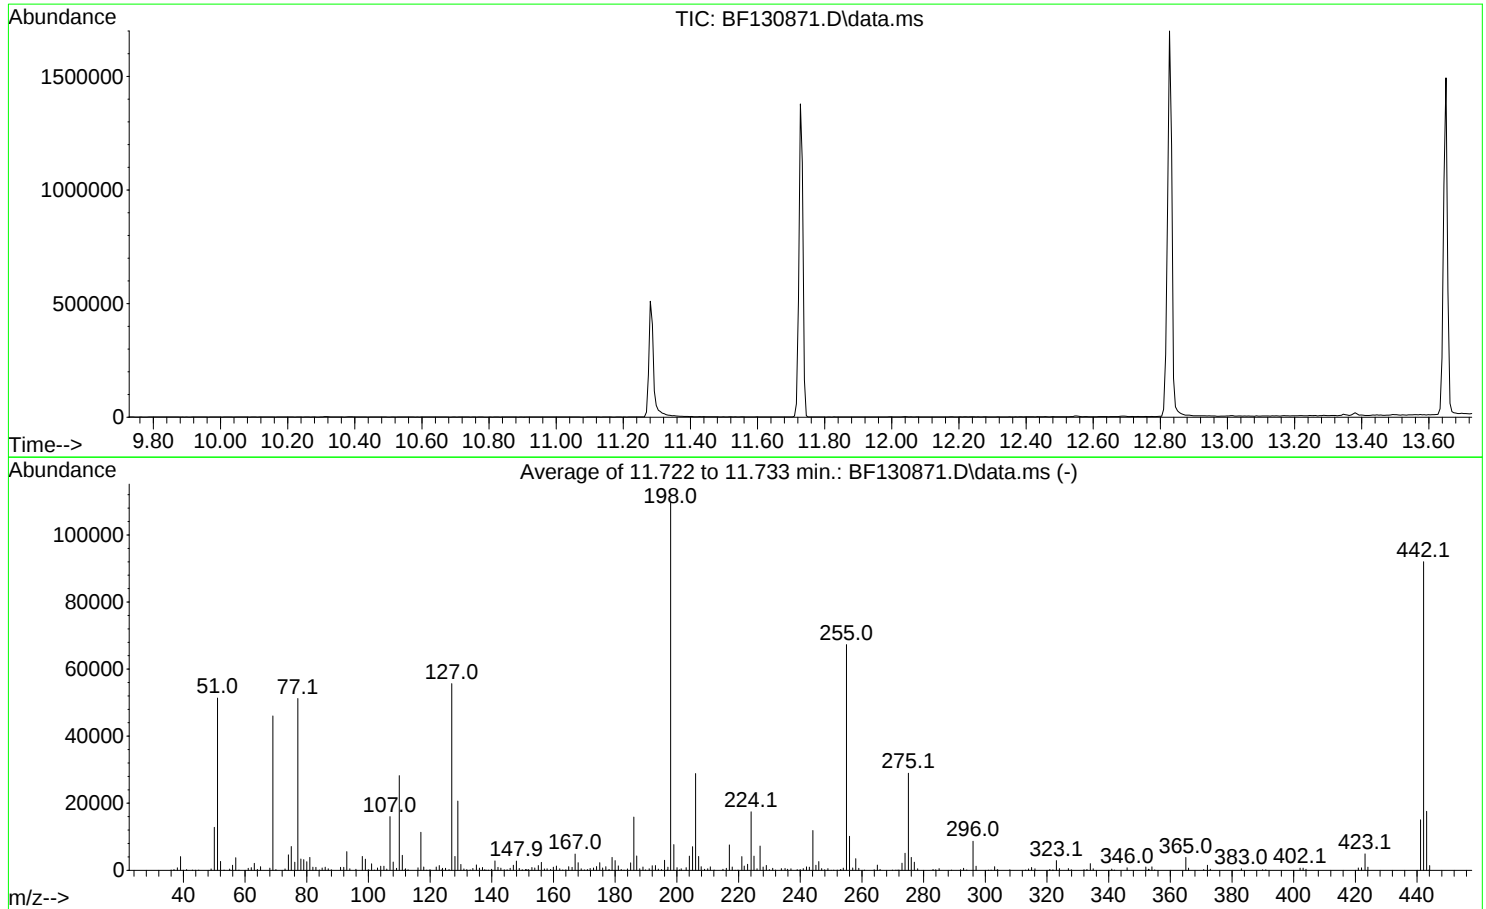




AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	51384	PASS
68	69	0.00	2	1.4	653	PASS
69	198	0.00	100	41.9	46019	PASS
70	69	0.00	2	0.4	204	PASS
127	198	10	80	50.7	55645	PASS
197	198	0.00	2	0.9	935	PASS
198	198	100	100	100.0	109707	PASS
199	198	5	9	7.0	7664	PASS
275	198	10	60	26.4	28928	PASS
365	198	1	100	3.5	3844	PASS
441	198	0.01	100	13.7	15080	PASS
442	442	50	100	100.0	92043	PASS
443	442	15	24	19.1	17573	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103122\
 Data File : BF130871.D
 Acq On : 31 Oct 2022 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 31 17:06:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 29 05:41:34 2022
 Response via : Initial Calibration

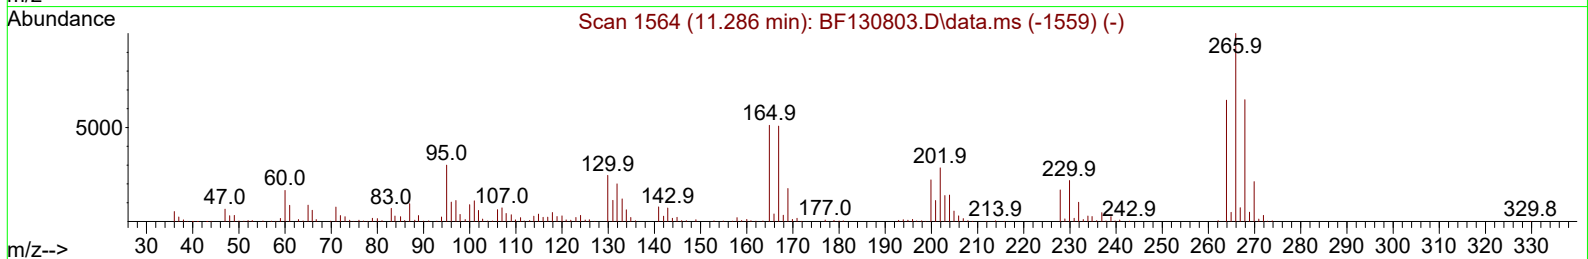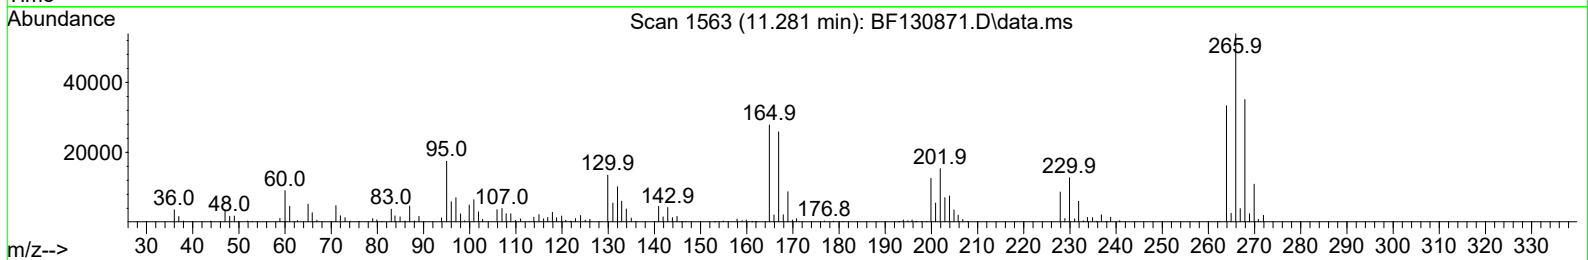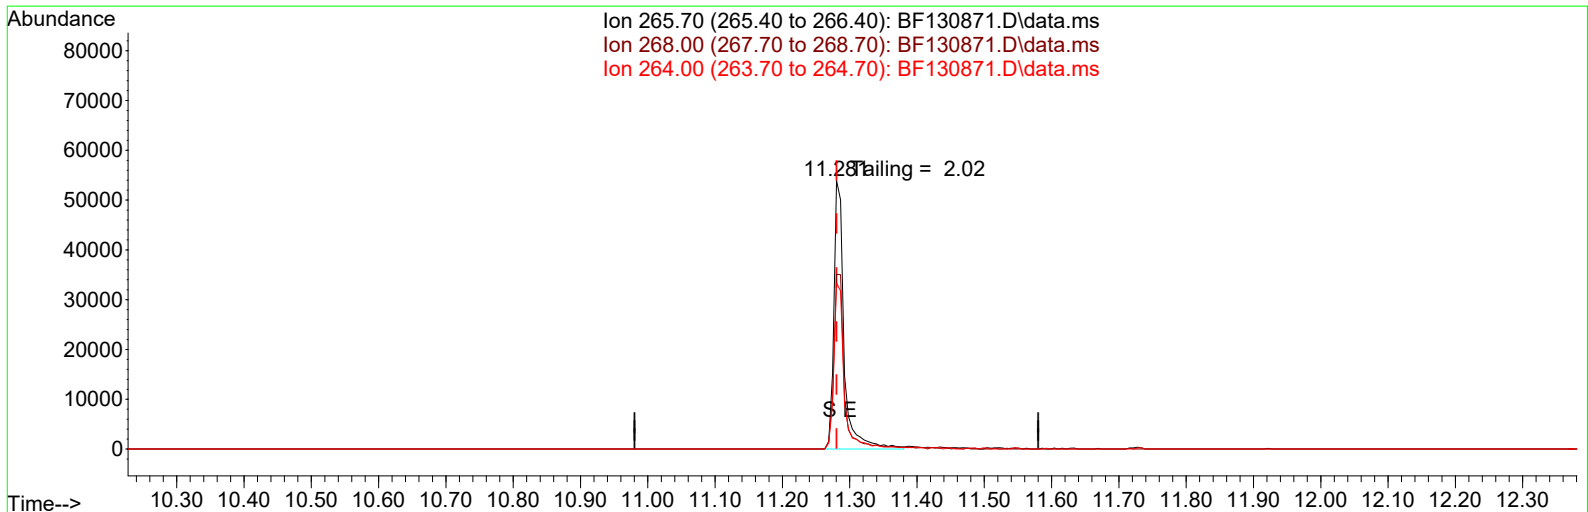

TIC: BF130871.D\data.ms

(70) Pentachlorophenol (C)

11.281min (+ 0.000) 18541.99 ng




response 56742

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	65.11
264.00	64.50	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103122\
Data File : BF130871.D
Acq On : 31 Oct 2022 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 17:06:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration

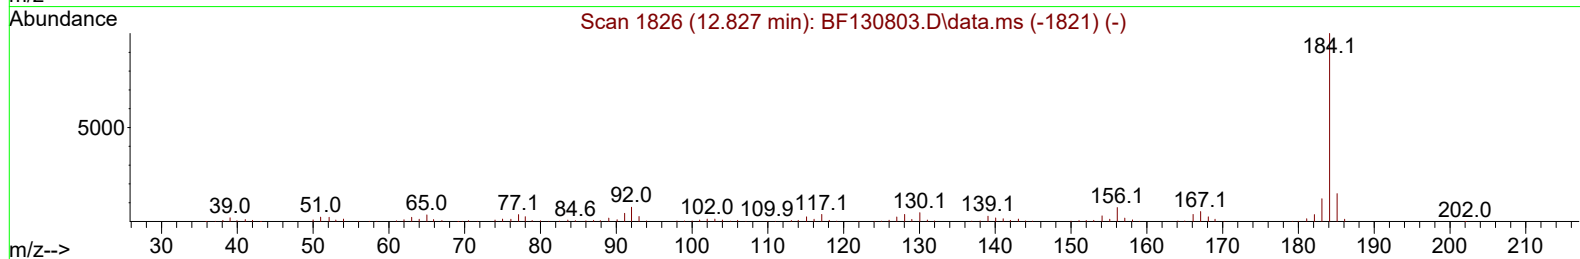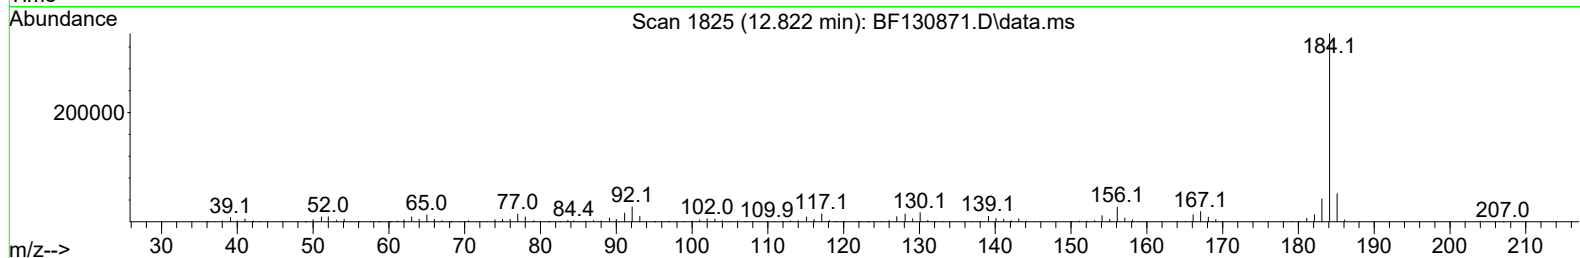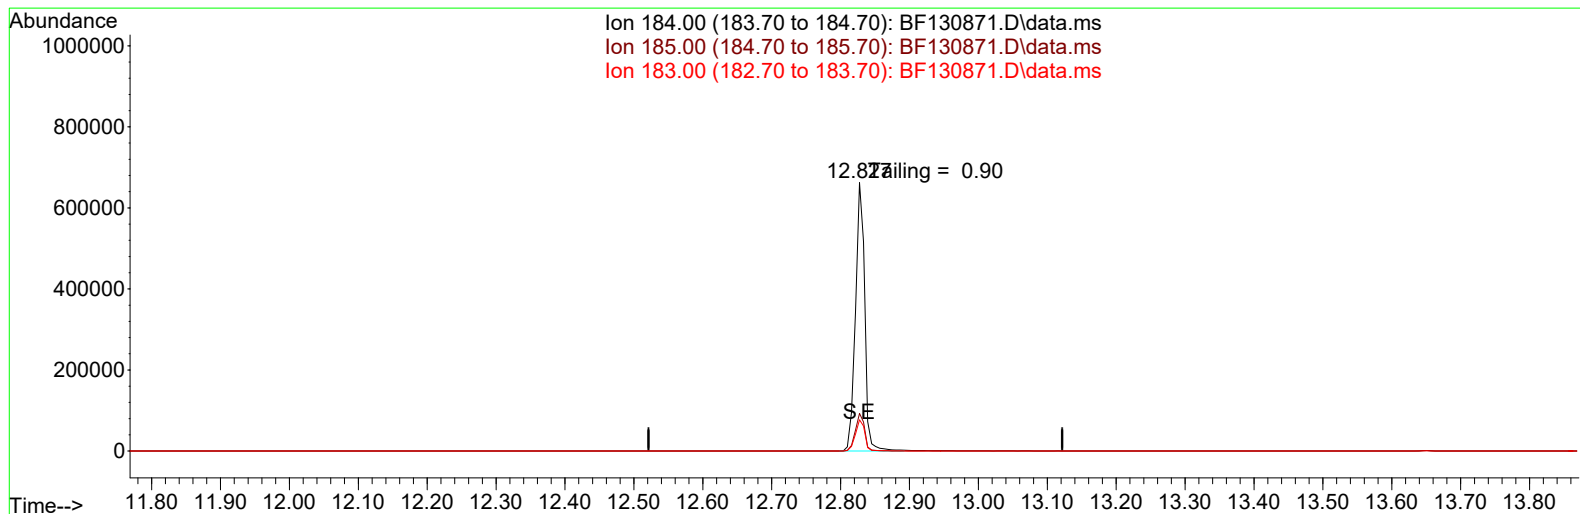

TIC: BF130871.D\data.ms

(77) Benzidine

12.822min (-12.822) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.80	0.00#
183.00	12.10	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2022	BNA_F	<u>BF130871.D</u>
Compound Name	Response	Retention Time
DDT	211017	13.651
DDD	3190	13.38
DDE	466	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3656	214673	1.70

Instrument :
BNA_F
ClientSampleId :
DFTPP