
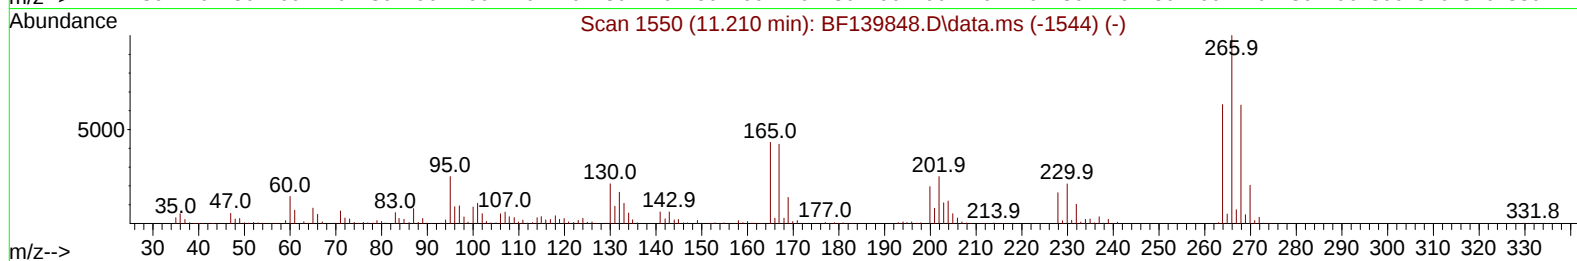
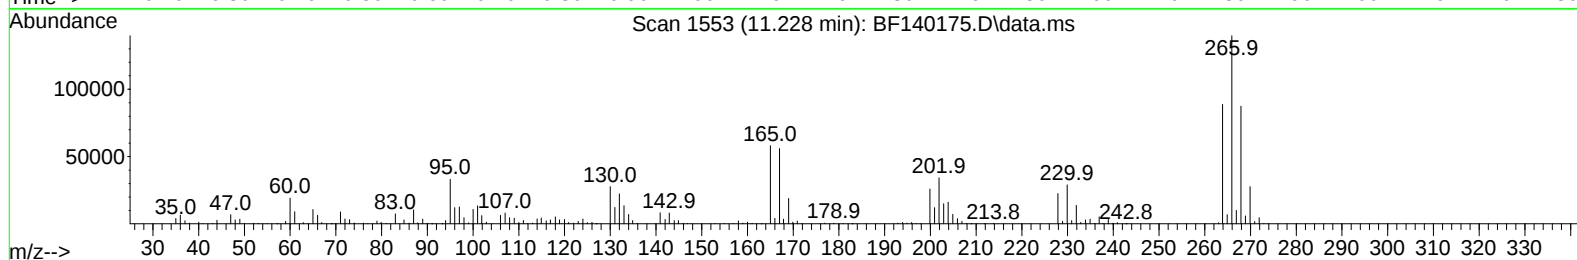


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140175.D
Acq On : 31 Oct 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 19:50:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

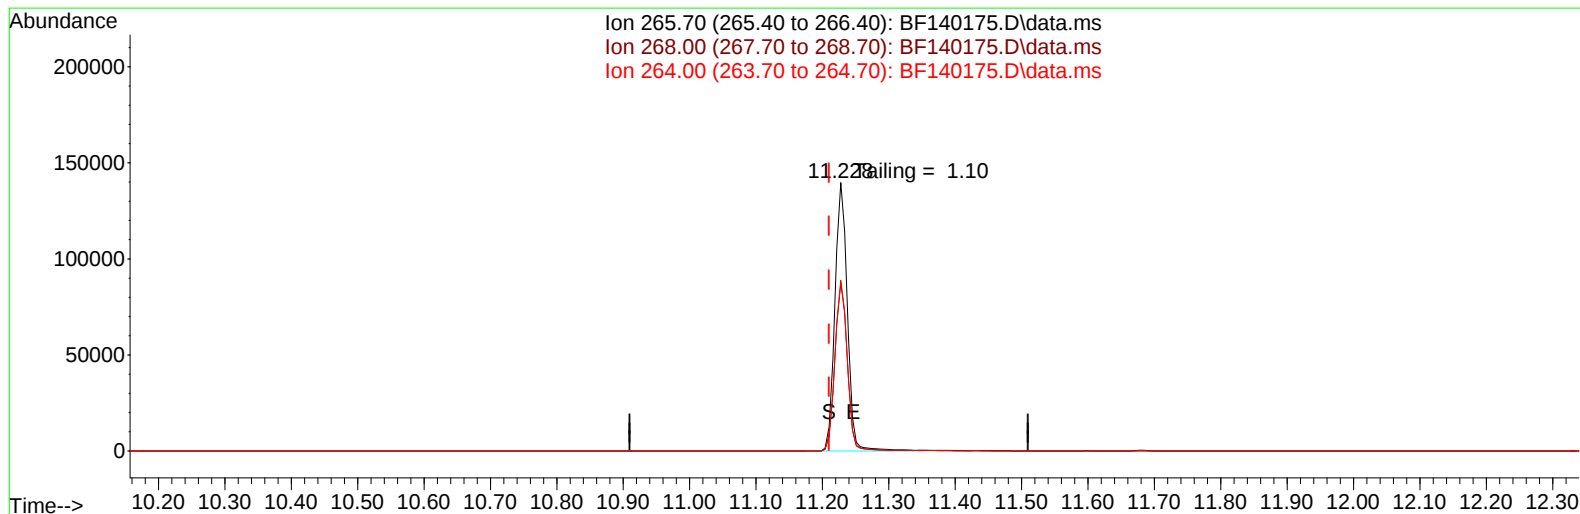

TIC: BF140175.D\data.ms

(70) Pentachlorophenol (C)




11.228min (+ 0.018) 96214.53 ng

response 181993

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.62
264.00	63.20	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140175.D
Acq On : 31 Oct 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 19:50:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

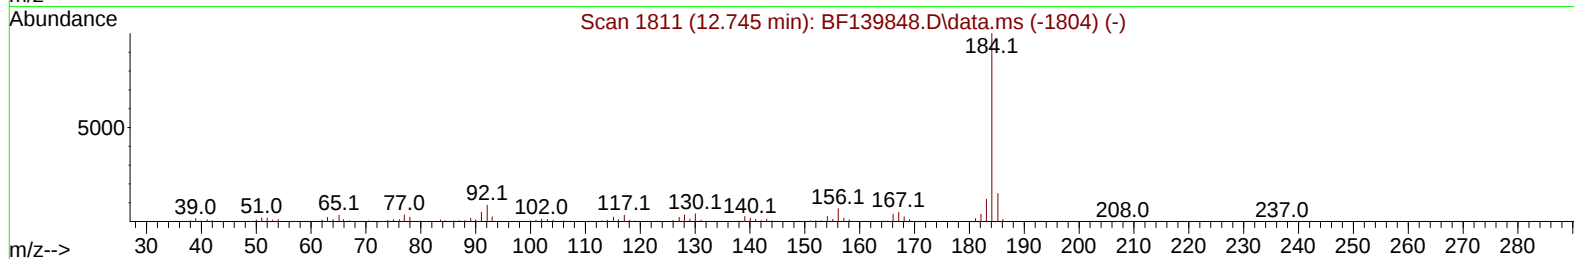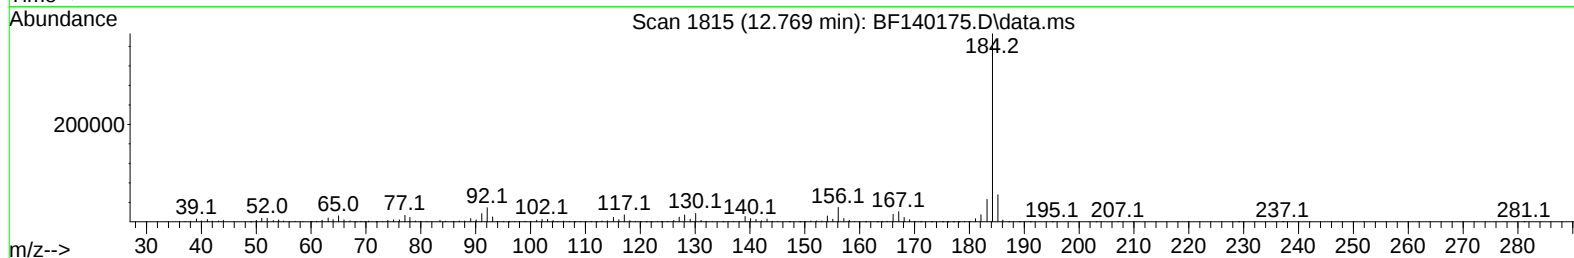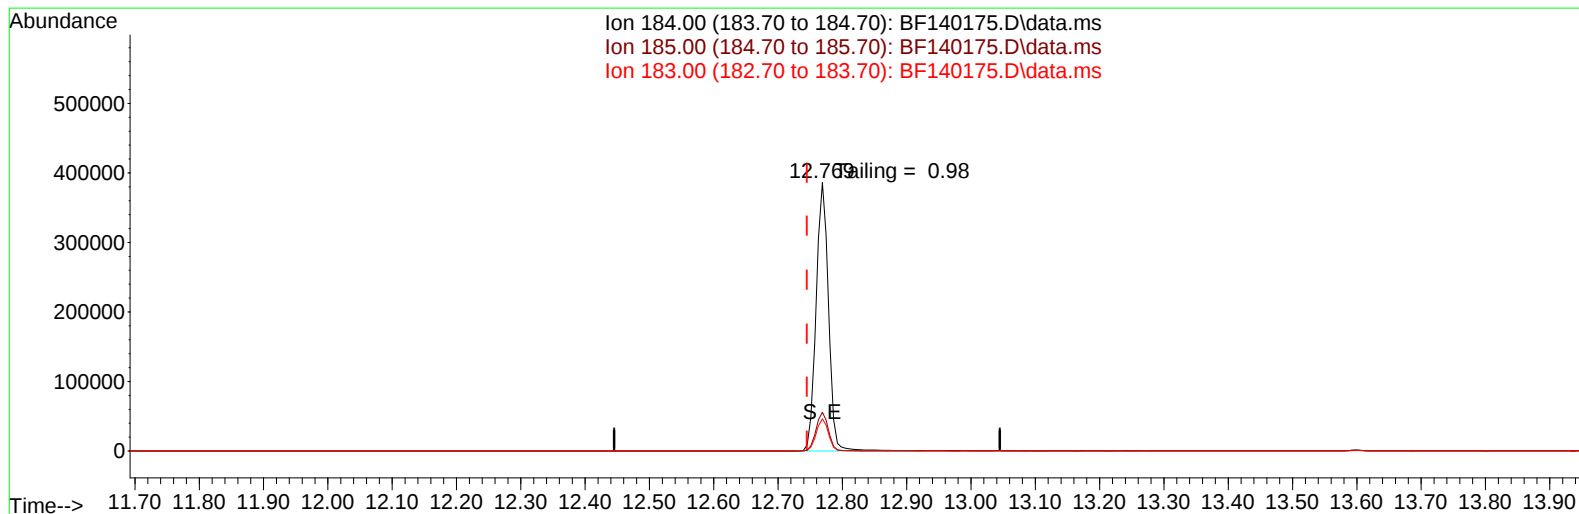

TIC: BF140175.D\data.ms

(77) Benzidine

12.769min (+ 0.024) 28582.51 ng

response 516523

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.45
183.00	11.80	11.98
0.00	0.00	0.00