

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
 Data File : BF140177.D
 Acq On : 31 Oct 2024 09:48
 Operator : RC/JU
 Sample : PB164540BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB164540BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	24	30	38	rVB	81725	136240	2.63%	0.475%
2	5.516	575	582	587	rBV	2500622	3549296	68.55%	12.383%
3	6.516	744	752	757	rBV	2312333	3629987	70.11%	12.665%
4	6.887	810	815	820	rVB	618992	755324	14.59%	2.635%
5	7.445	903	910	915	rBV	1720333	2459897	47.51%	8.583%
6	8.163	1026	1032	1038	rBV	753723	997696	19.27%	3.481%
7	9.245	1208	1216	1221	rBV	3127088	4479727	86.52%	15.630%
8	9.928	1325	1332	1337	rBV	904300	1175632	22.71%	4.102%
9	10.722	1459	1467	1485	rBV	2169249	2996392	57.87%	10.454%
10	11.422	1580	1586	1591	rBV	1016220	1276274	24.65%	4.453%
11	13.021	1851	1858	1863	rBV	3704578	5177405	100.00%	18.064%
12	14.092	2034	2040	2047	rBV	841043	1126446	21.76%	3.930%
13	15.633	2296	2302	2314	rVB	535077	901180	17.41%	3.144%




Sum of corrected areas: 28661496

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140177.D
Acq On : 31 Oct 2024 09:48
Operator : RC/JU
Sample : PB164540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164540BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

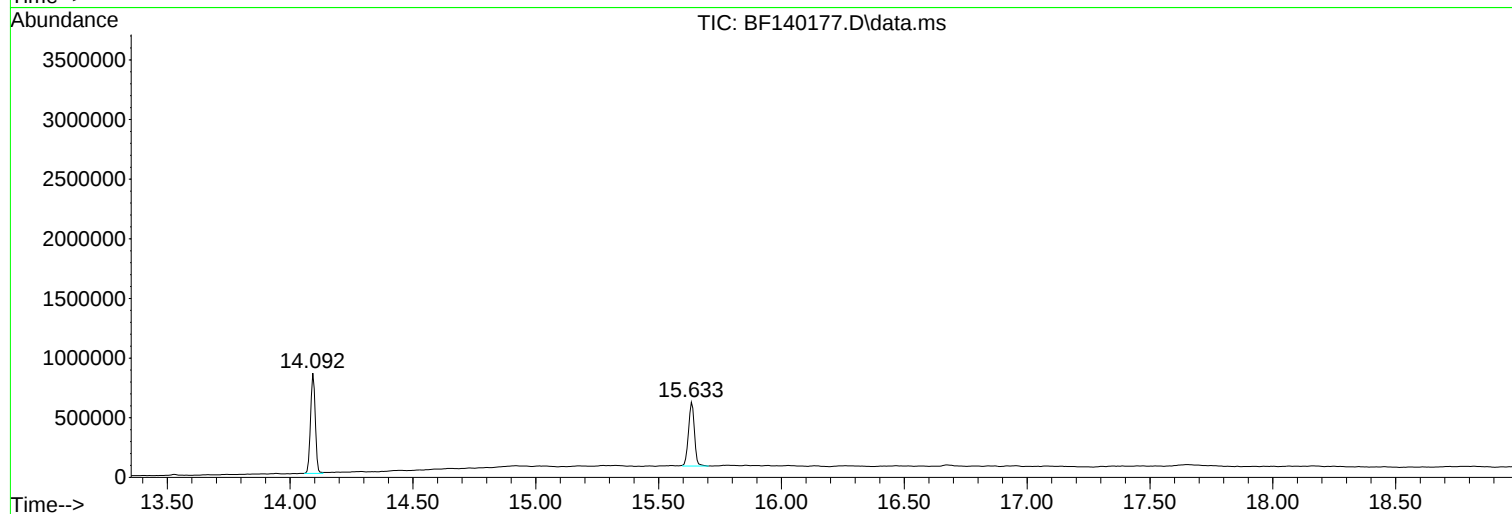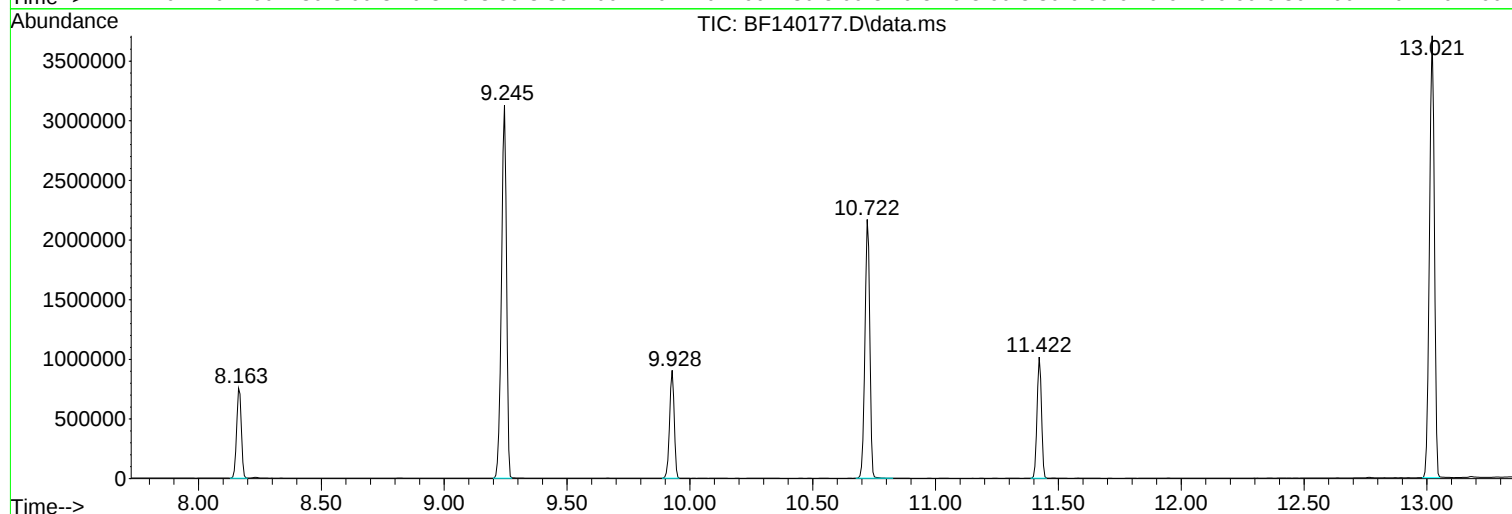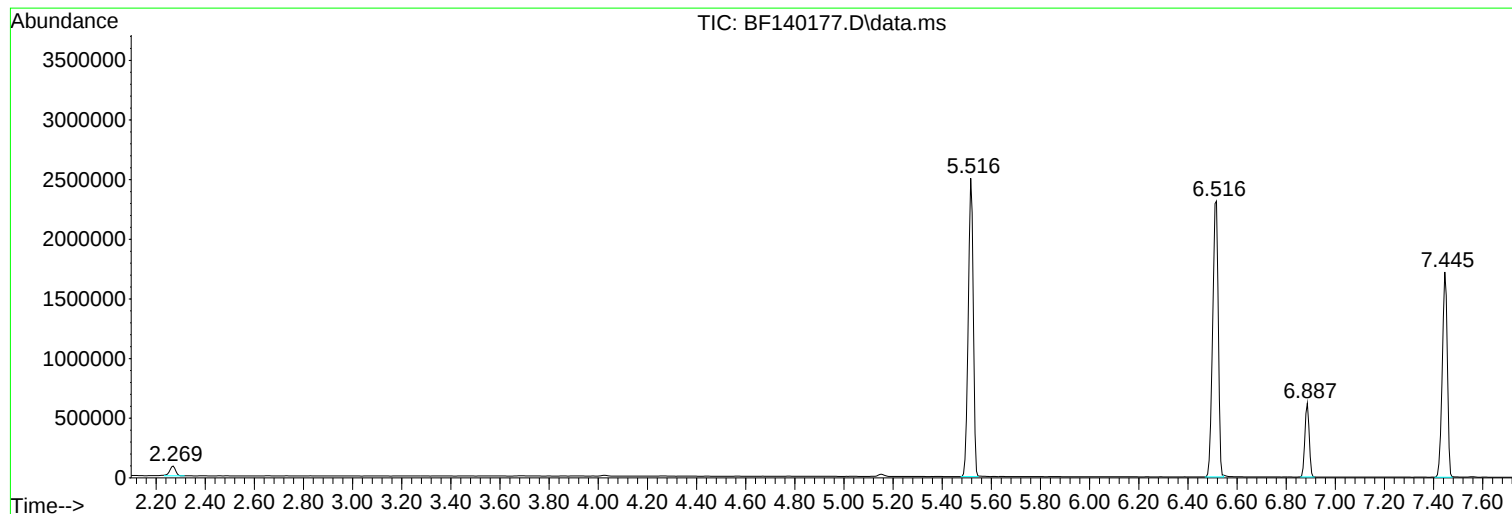

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140177.D
Acq On : 31 Oct 2024 09:48
Operator : RC/JU
Sample : PB164540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164540BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.269	3.61 ng	136240	1,4-Dichlorobenzene-d4	6.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	37
4			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23
5			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17

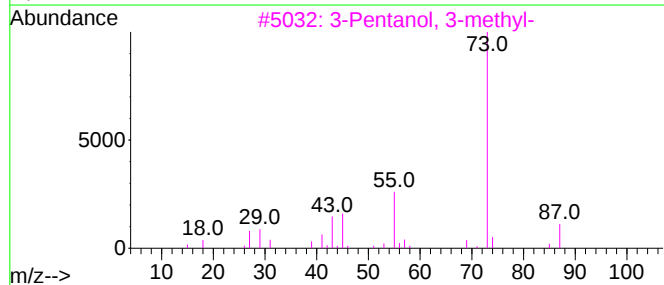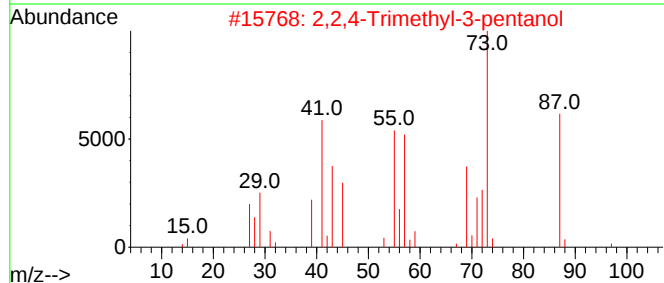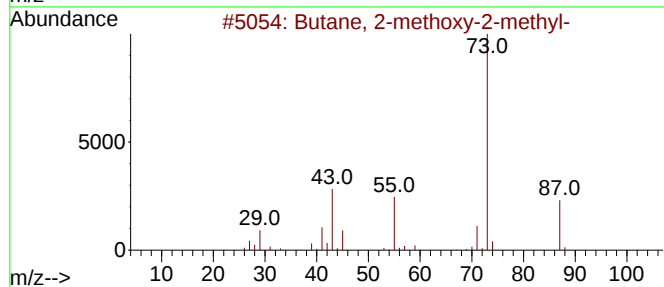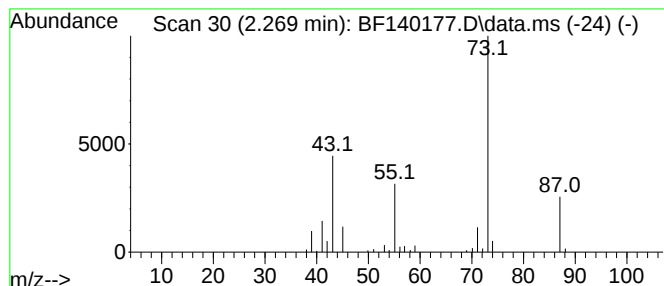

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140177.D
Acq On : 31 Oct 2024 09:48
Operator : RC/JU
Sample : PB164540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164540BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.269	3.6	ng	136240	1	6.887	755324	20.0