

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
 Data File : BF140184.D
 Acq On : 31 Oct 2024 13:03
 Operator : RC/JU
 Sample : P4611-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	5	12	20	rVB	1240902	1999812	69.64%	9.141%
2	5.504	573	580	585	rBV	1602073	2180147	75.92%	9.965%
3	6.504	744	750	756	rBV	1607439	2293926	79.89%	10.485%
4	6.887	809	815	820	rVB	476919	608322	21.19%	2.780%
5	7.445	903	910	915	rBV	1140953	1552987	54.08%	7.098%
6	7.692	948	952	959	rVB	41201	51080	1.78%	0.233%
7	8.163	1025	1032	1040	rBV	655274	846655	29.49%	3.870%
8	8.375	1064	1068	1076	rVB2	21495	28994	1.01%	0.133%
9	9.239	1209	1215	1221	rBV	2145798	2871462	100.00%	13.125%
10	9.928	1323	1332	1337	rBV	732422	956591	33.31%	4.372%
11	10.639	1448	1453	1460	rBV	265857	342304	11.92%	1.565%
12	10.716	1460	1466	1477	rVV	1360706	1788888	62.30%	8.177%
13	10.833	1480	1486	1494	rVB2	19433	35475	1.24%	0.162%
14	11.416	1580	1585	1593	rBV	706753	944171	32.88%	4.316%
15	11.951	1668	1676	1686	rBV	536388	821379	28.60%	3.754%
16	12.198	1714	1718	1724	rBV2	25732	42618	1.48%	0.195%
17	12.639	1788	1793	1804	rBV	46642	86774	3.02%	0.397%
18	12.733	1805	1809	1822	rBV	112444	185396	6.46%	0.847%
19	12.869	1827	1832	1838	rVB	34470	59023	2.06%	0.270%
20	13.010	1851	1856	1862	rBV	1767700	2332719	81.24%	10.662%
21	13.557	1944	1949	1953	rBV	192825	254339	8.86%	1.163%
22	13.927	2007	2012	2023	rBV2	156001	281818	9.81%	1.288%
23	14.080	2032	2038	2051	rBV	438668	681991	23.75%	3.117%
24	14.580	2120	2123	2137	rVB3	23907	53054	1.85%	0.242%
25	15.168	2219	2223	2232	rVB	43196	90737	3.16%	0.415%
26	15.615	2293	2299	2304	rBV	299877	487505	16.98%	2.228%




Sum of corrected areas: 21878167

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140184.D
Acq On : 31 Oct 2024 13:03
Operator : RC/JU
Sample : P4611-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

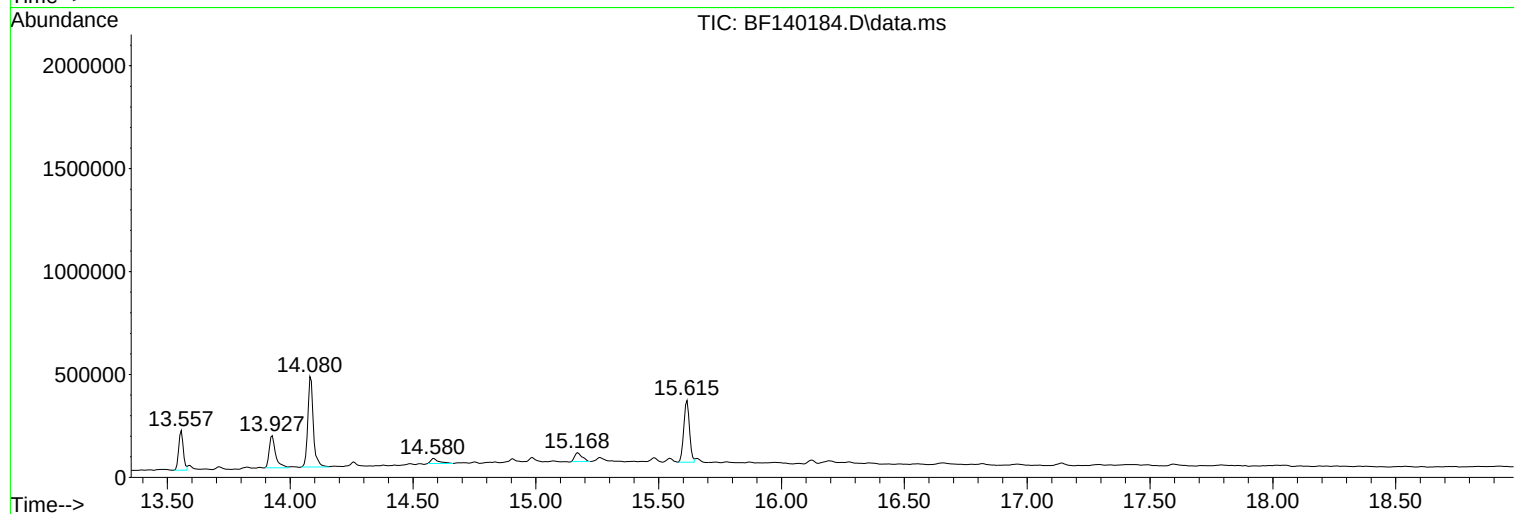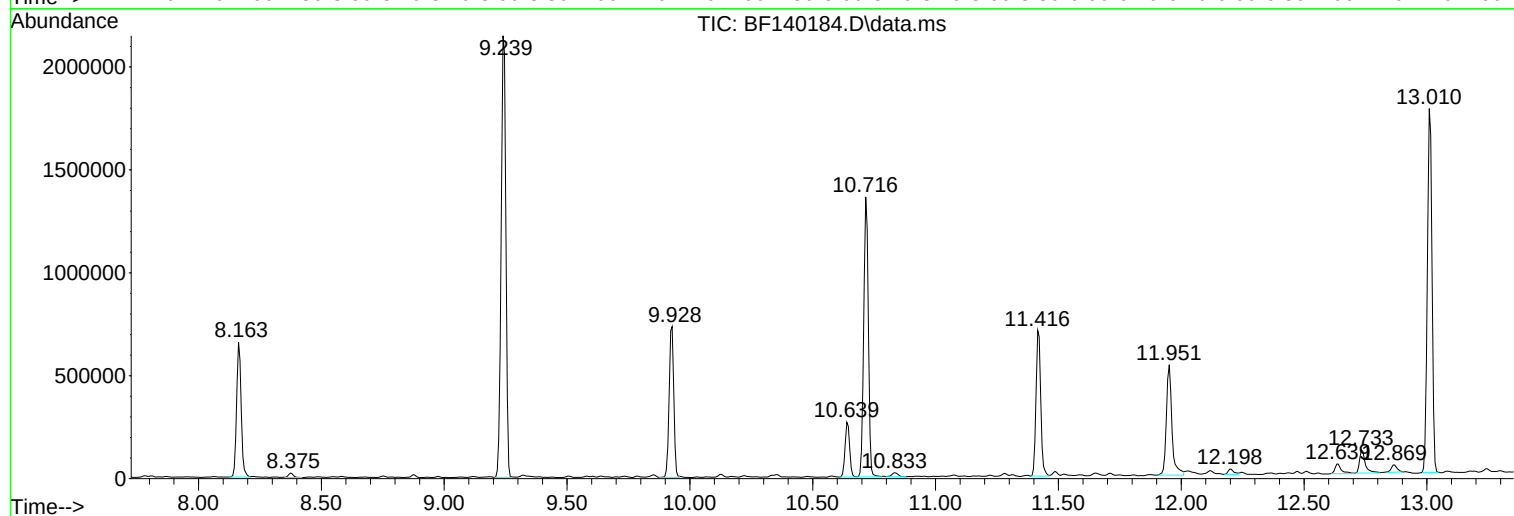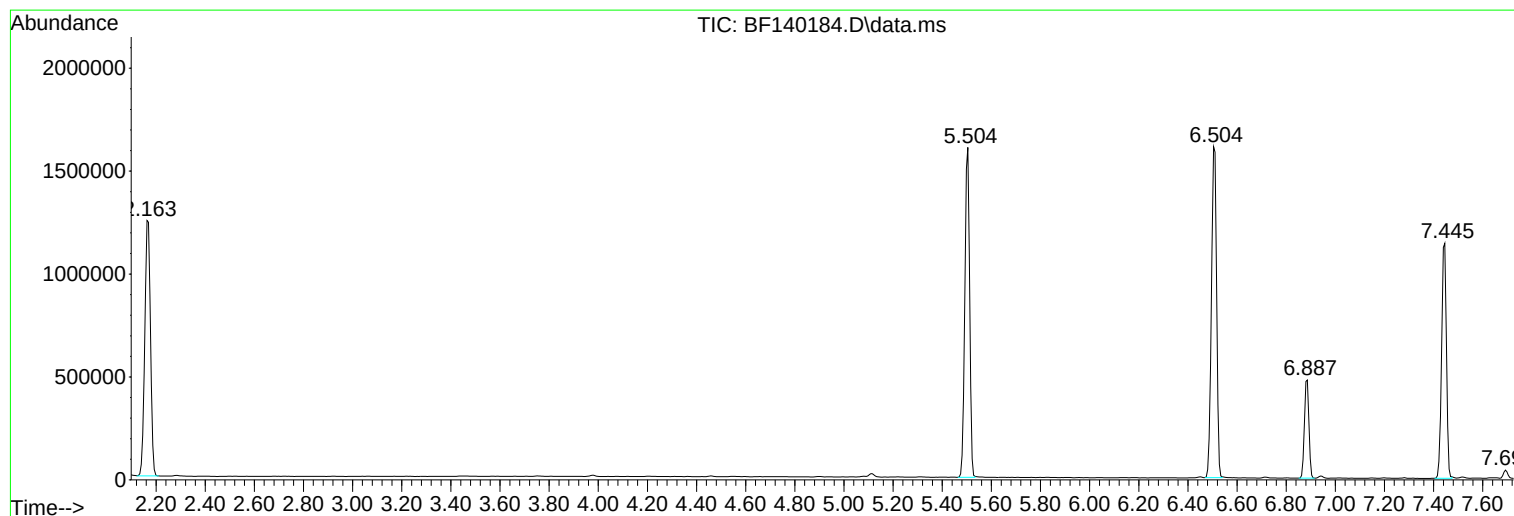

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140184.D
Acq On : 31 Oct 2024 13:03
Operator : RC/JU
Sample : P4611-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140184.D
Acq On : 31 Oct 2024 13:03
Operator : RC/JU
Sample : P4611-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc