
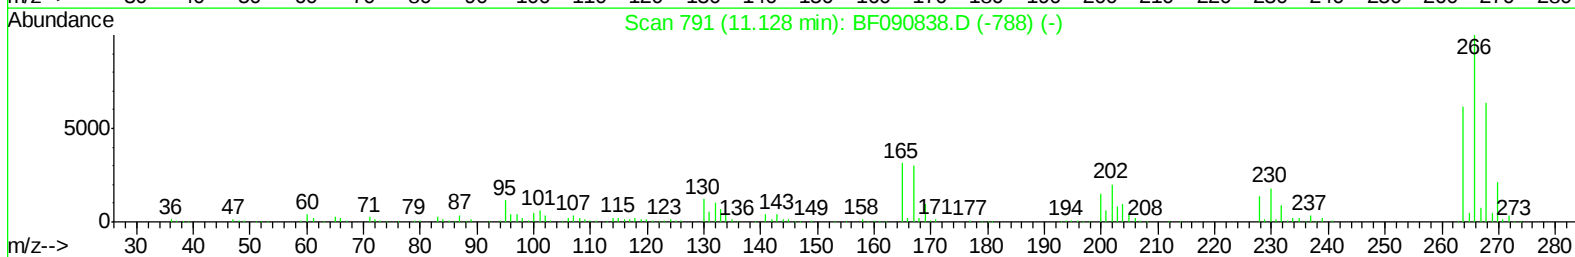
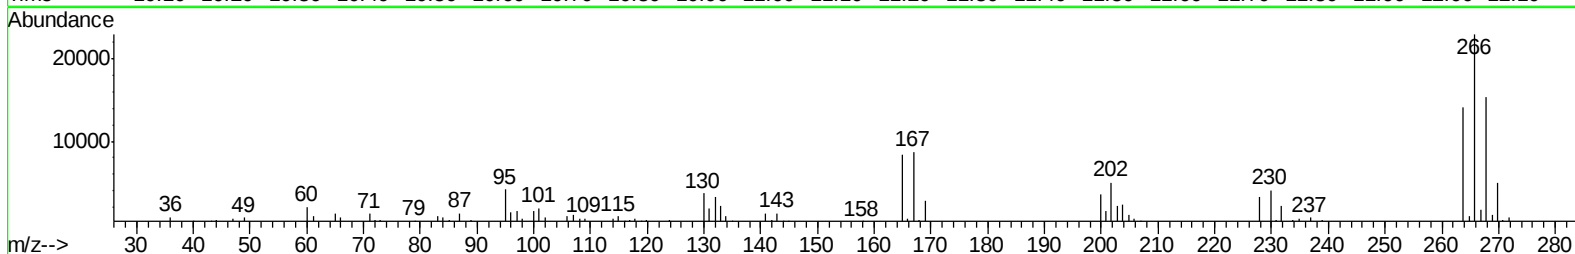


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110116\
Data File : BF090947.D
Acq On : 1 Nov 2016 13:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:13:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 11:53:50 2016
Response via : Initial Calibration

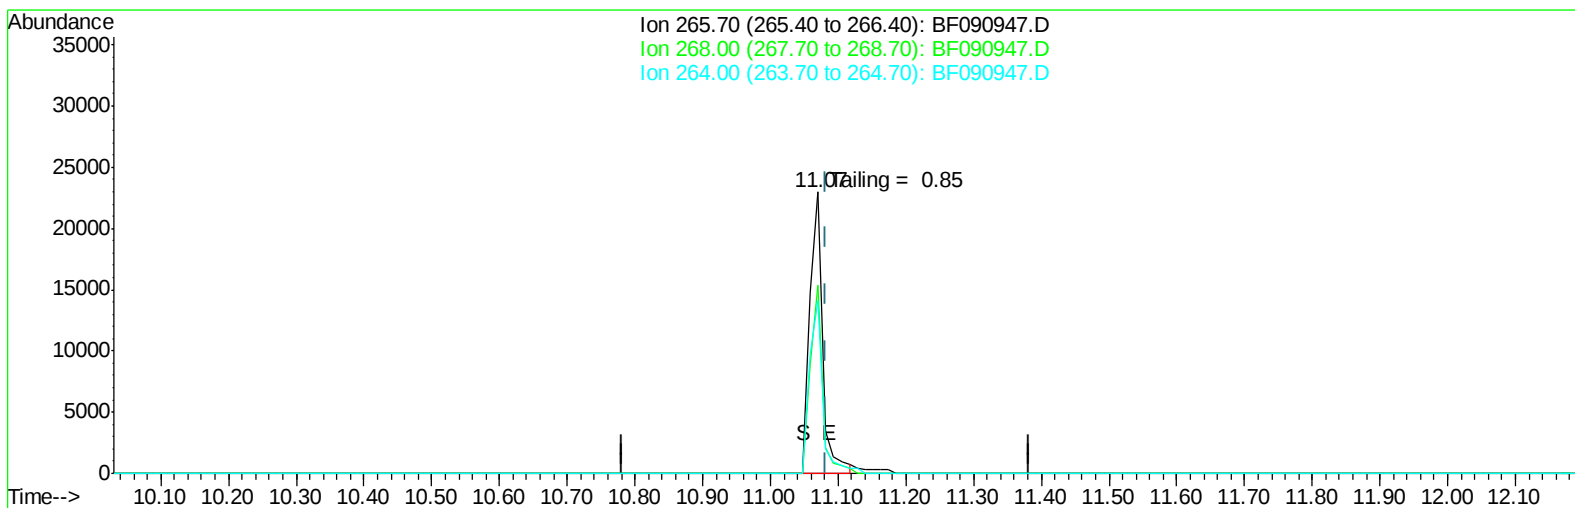

TIC: BF090947.D

(69) Pentachlorophenol (C)




11.071min (-0.011) 0.00ng

response 31553

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	67.01
264.00	62.70	61.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110116\
Data File : BF090947.D
Acq On : 1 Nov 2016 13:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:13:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 11:53:50 2016
Response via : Initial Calibration

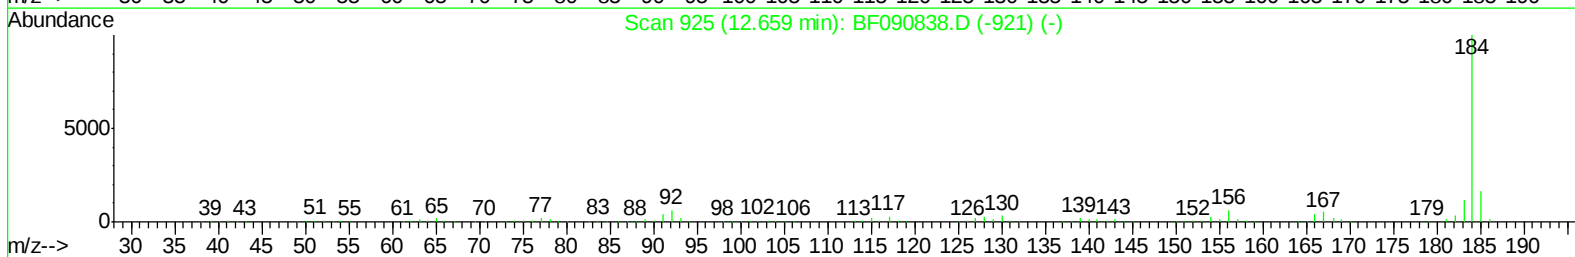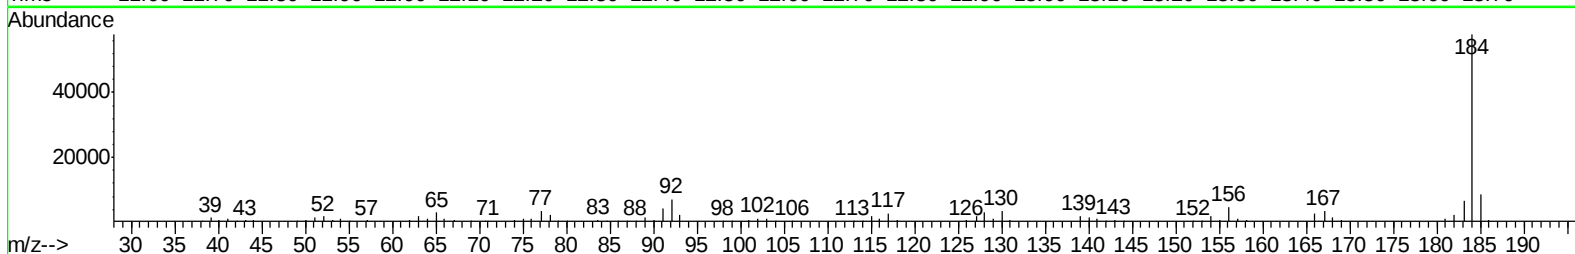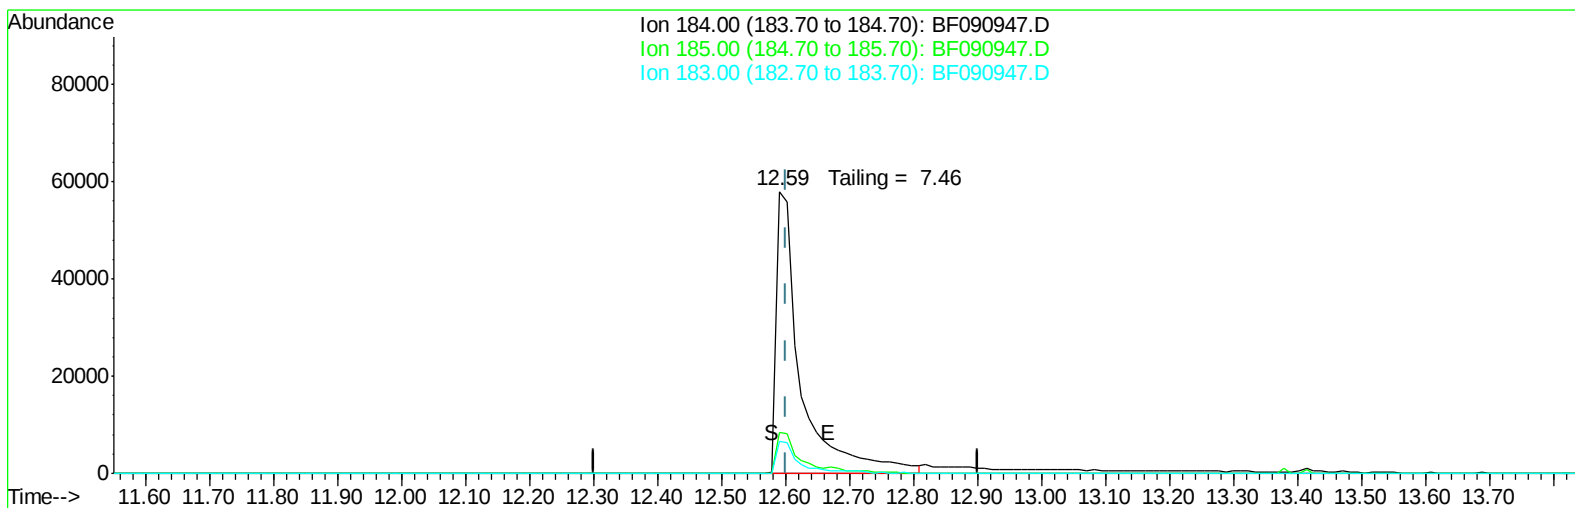

TIC: BF090947.D

(76) Benzidine

12.591min (-0.011) 21102.14ng

response 154816

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.71
183.00	9.50	11.17
0.00	0.00	0.00