


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110116\
 Data File : BF090947.D
 Acq On : 1 Nov 2016 13:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 01 11:53:50 2016

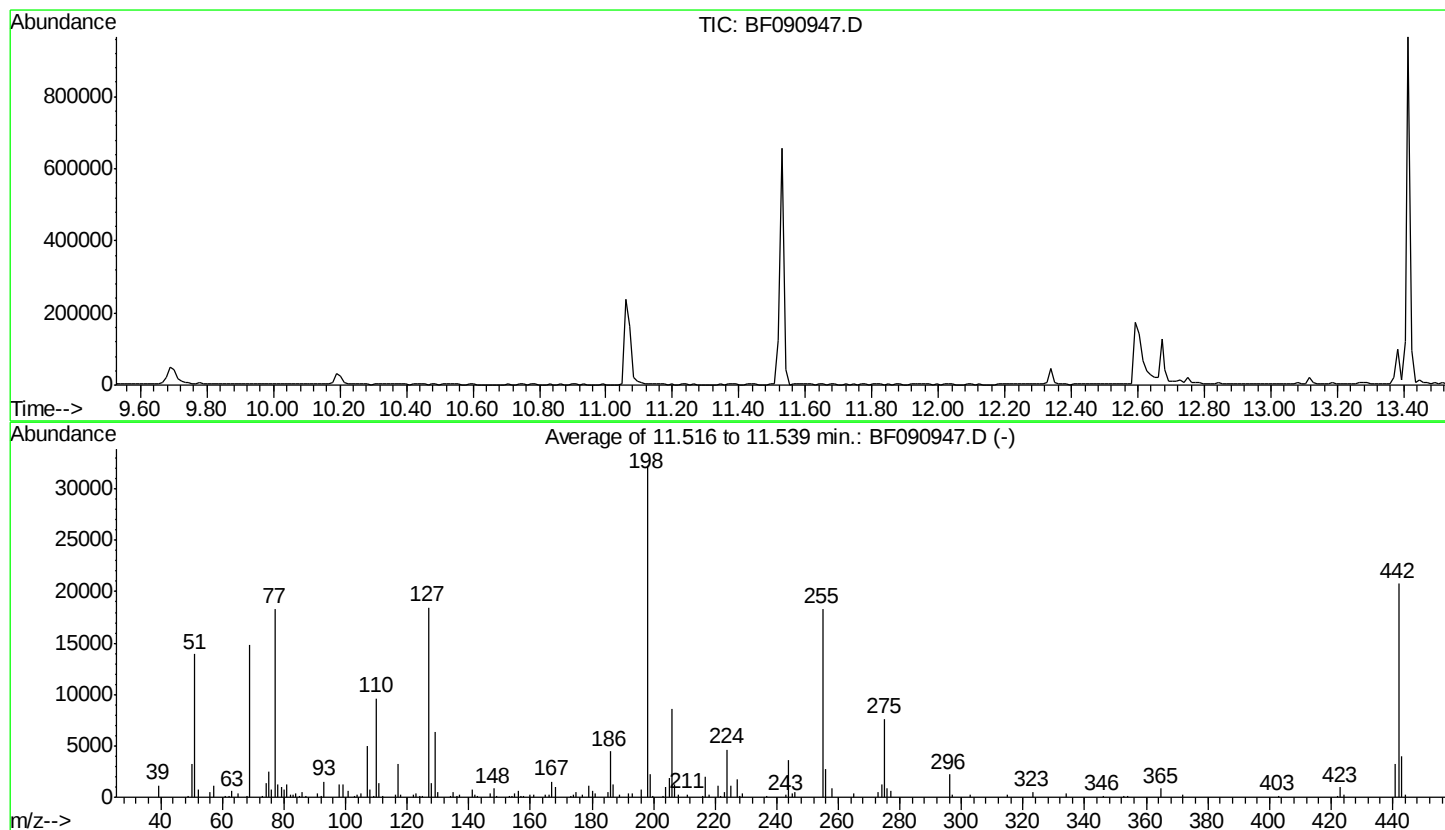

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	13906	PASS
68	69	0.00	2	1.0	144	PASS
69	198	0.00	100	46.0	14853	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.3	18494	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32267	PASS
199	198	5	9	6.8	2194	PASS
275	198	10	60	23.7	7632	PASS
365	198	1	100	2.6	839	PASS
441	442	0.01	24	15.3	3182	PASS
442	198	50	100	64.4	20776	PASS
443	442	15	24	19.1	3962	PASS