


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110117\
 Data File : BF100043.D
 Acq On : 1 Nov 2017 14:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 01 18:13:08 2017

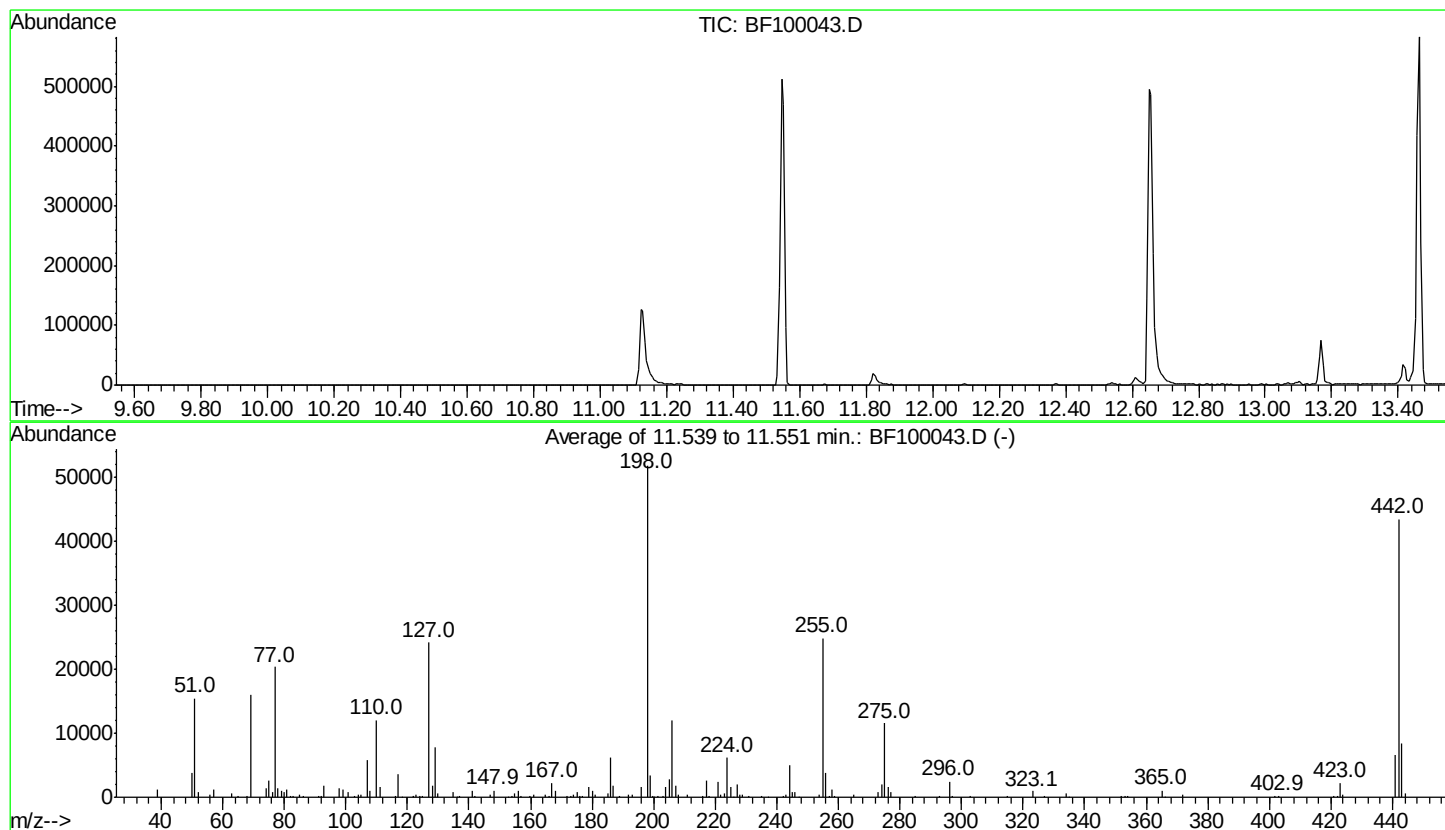

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	15473	PASS
68	69	0.00	2	1.8	281	PASS
69	198	0.00	100	30.7	15921	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	24119	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51800	PASS
199	198	5	9	6.6	3398	PASS
275	198	10	60	22.3	11545	PASS
365	198	1	100	2.0	1056	PASS
441	443	0.01	100	78.8	6698	PASS
442	198	50	100	83.8	43404	PASS
443	442	15	24	19.6	8500	PASS