


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110117\
 Data File : BF100068.D
 Acq On : 2 Nov 2017 2:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 01 18:13:08 2017

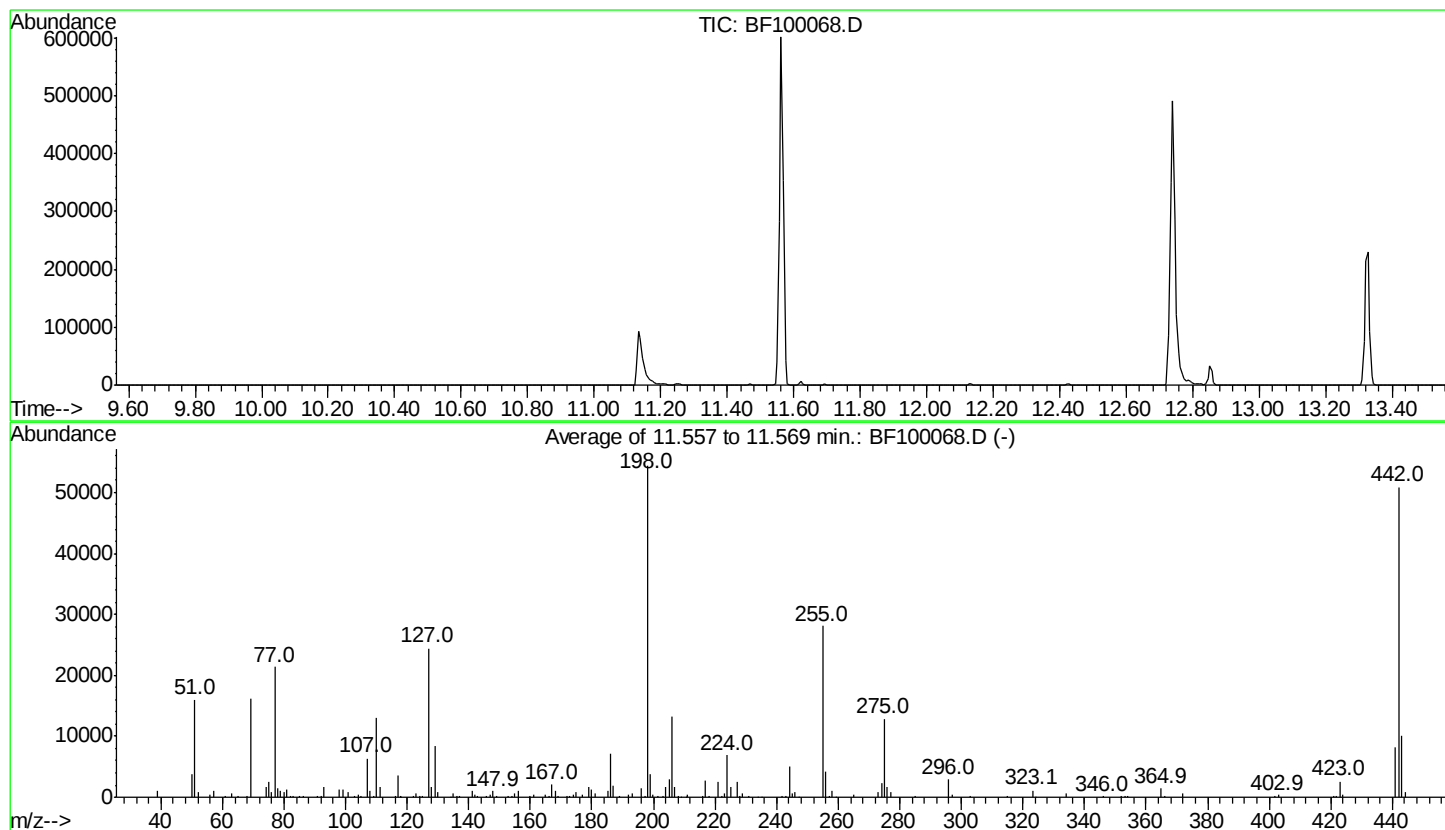

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	15979	PASS
68	69	0.00	2	1.4	219	PASS
69	198	0.00	100	29.7	16161	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	24469	PASS
197	198	0.00	2	0.4	209	PASS
198	198	100	100	100.0	54400	PASS
199	198	5	9	6.8	3710	PASS
275	198	10	60	23.6	12854	PASS
365	198	1	100	2.5	1373	PASS
441	443	0.01	100	82.7	8282	PASS
442	198	50	100	93.4	50832	PASS
443	442	15	24	19.7	10020	PASS