
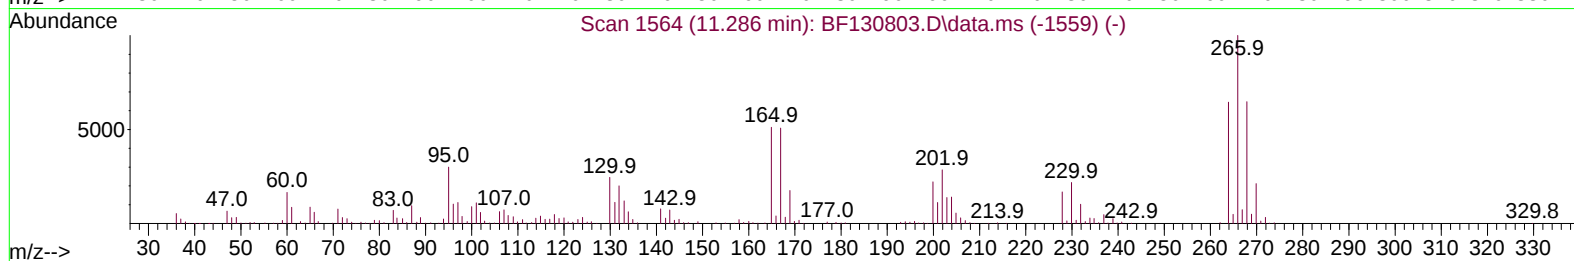
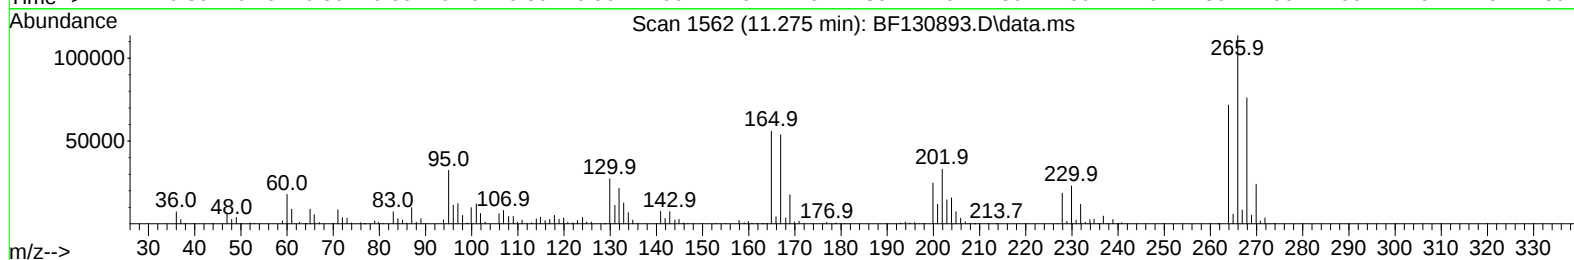


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
Data File : BF130893.D
Acq On : 01 Nov 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 10:51:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 08:18:35 2022
Response via : Initial Calibration

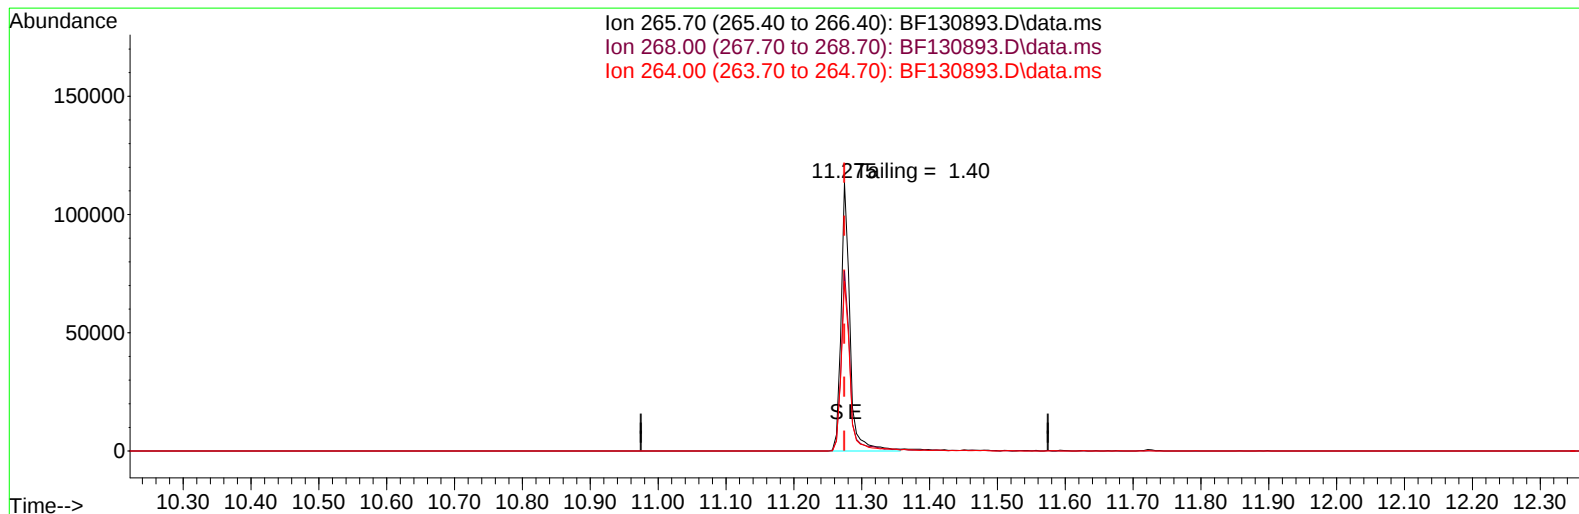

TIC: BF130893.D\data.ms

(70) Pentachlorophenol (C)




11.275min (+ 0.000) 21286.44 ng

response 102556

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.03
264.00	64.50	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
Data File : BF130893.D
Acq On : 01 Nov 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 10:51:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 08:18:35 2022
Response via : Initial Calibration

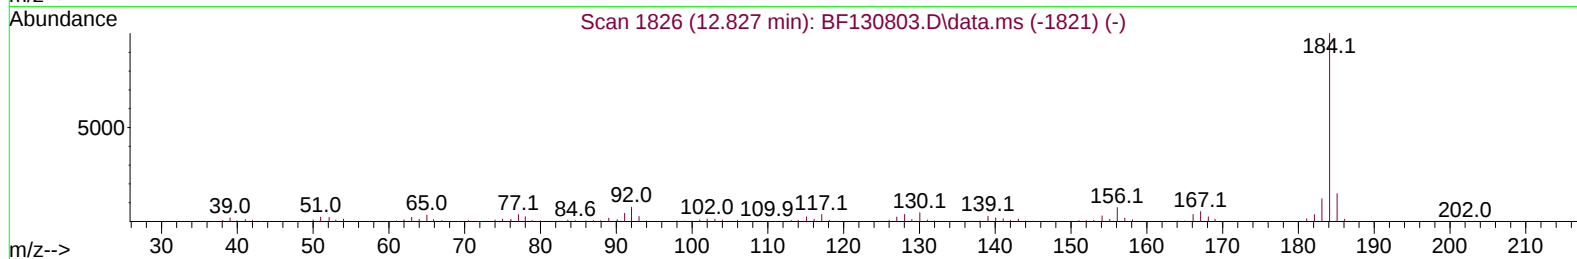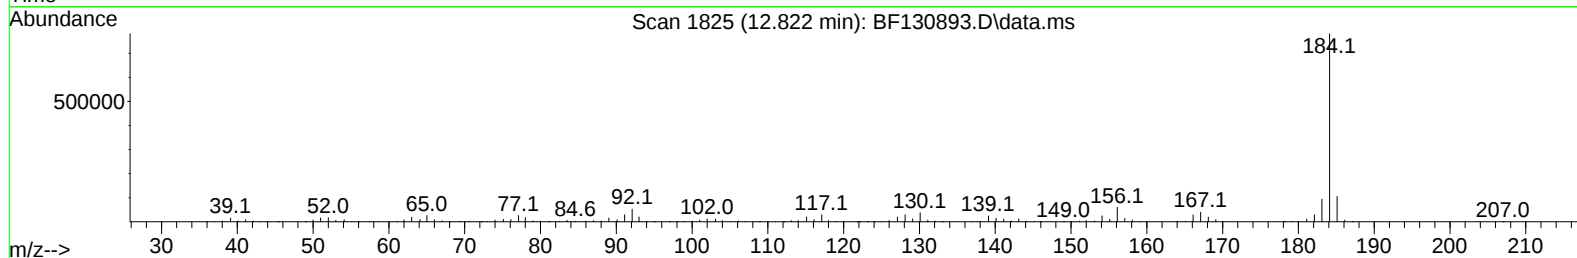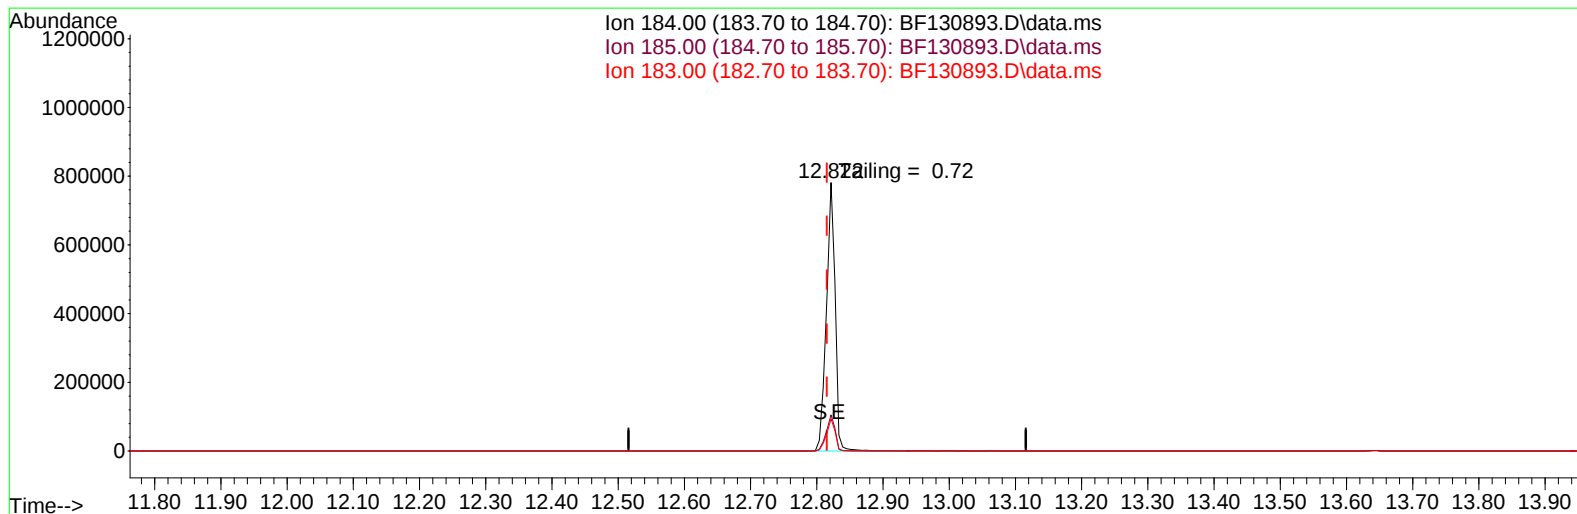

TIC: BF130893.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 392642.27 ng

response 724384

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.50
183.00	12.10	12.00
0.00	0.00	0.00