


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
 Data File : BF130893.D
 Acq On : 01 Nov 2022 10:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:46:02 2022

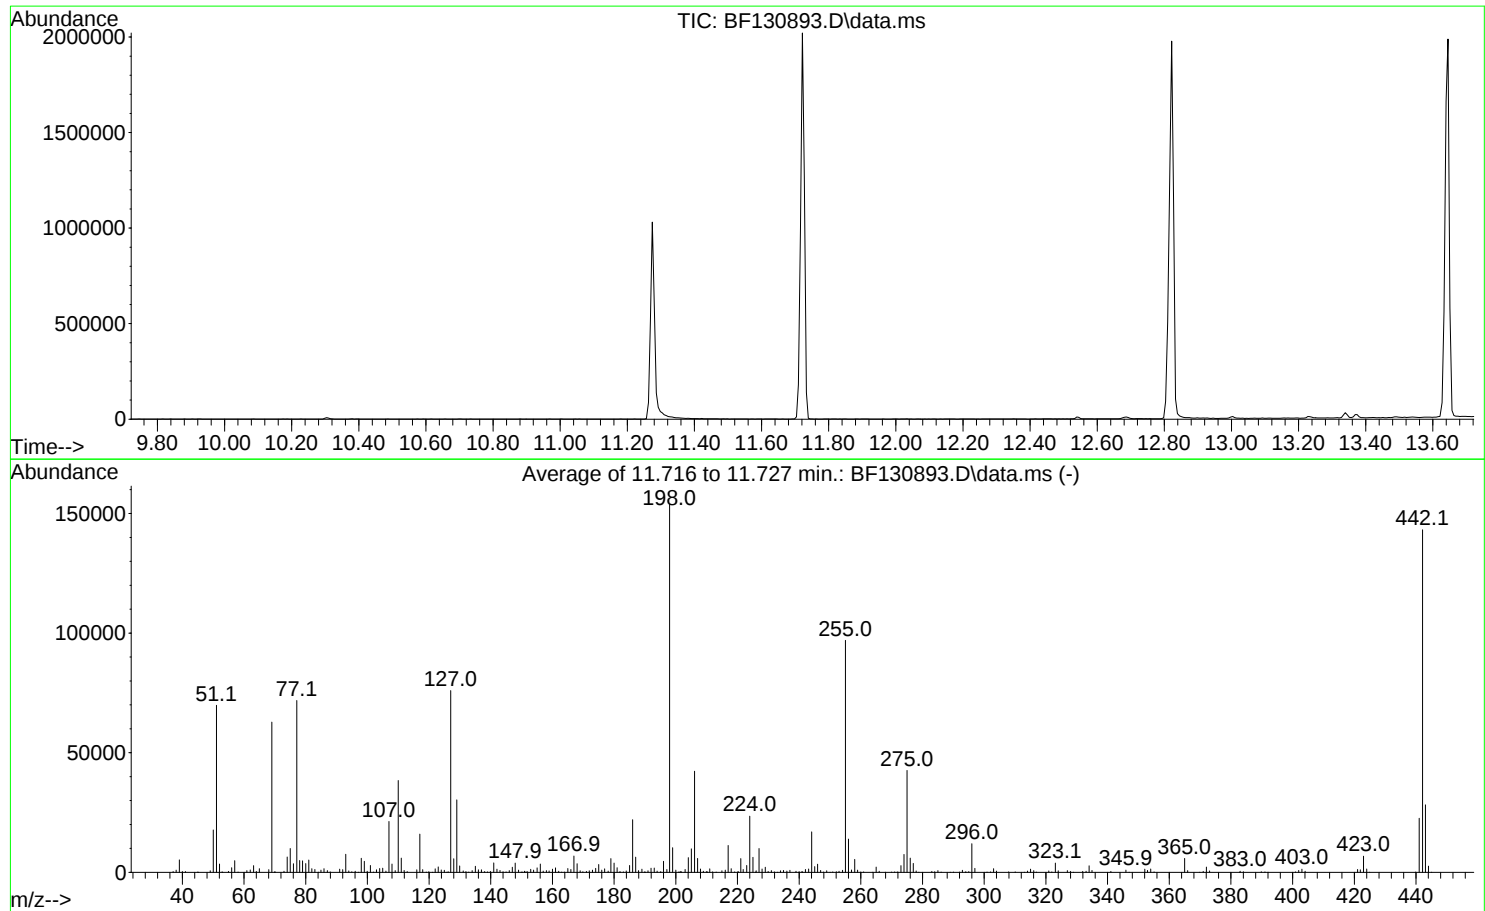




AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	69819	PASS
68	69	0.00	2	1.8	1140	PASS
69	198	0.00	100	40.8	62771	PASS
70	69	0.00	2	0.3	195	PASS
127	198	10	80	49.4	75984	PASS
197	198	0.00	2	0.7	1145	PASS
198	198	100	100	100.0	153811	PASS
199	198	5	9	6.7	10310	PASS
275	198	10	60	27.7	42592	PASS
365	198	1	100	3.8	5788	PASS
441	198	0.01	100	14.7	22560	PASS
442	442	50	100	100.0	143181	PASS
443	442	15	24	19.7	28219	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
Data File : BF130893.D
Acq On : 01 Nov 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 02 10:51:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 08:18:35 2022
Response via : Initial Calibration

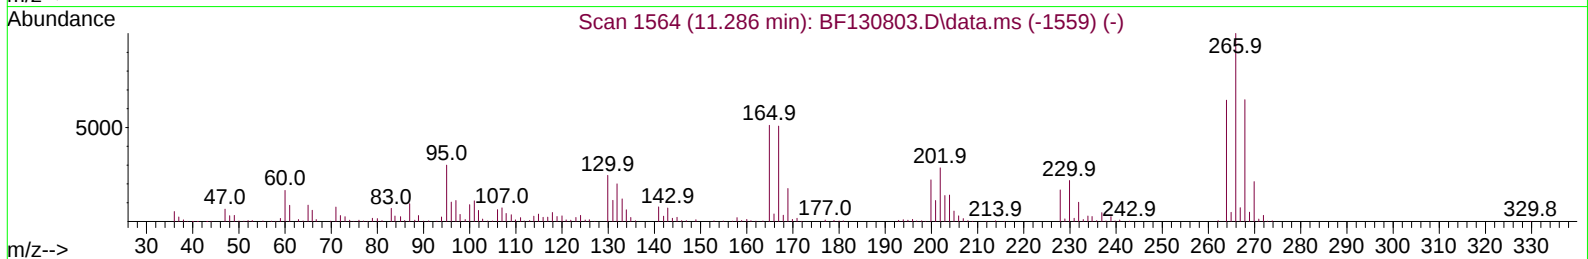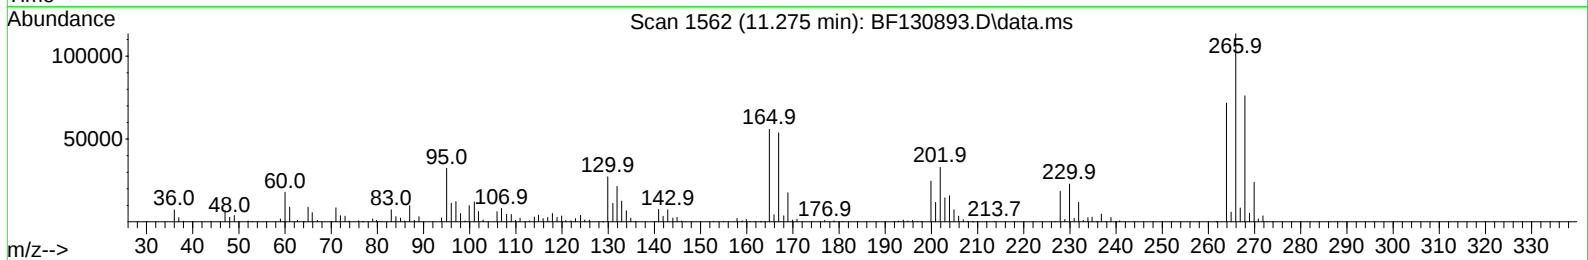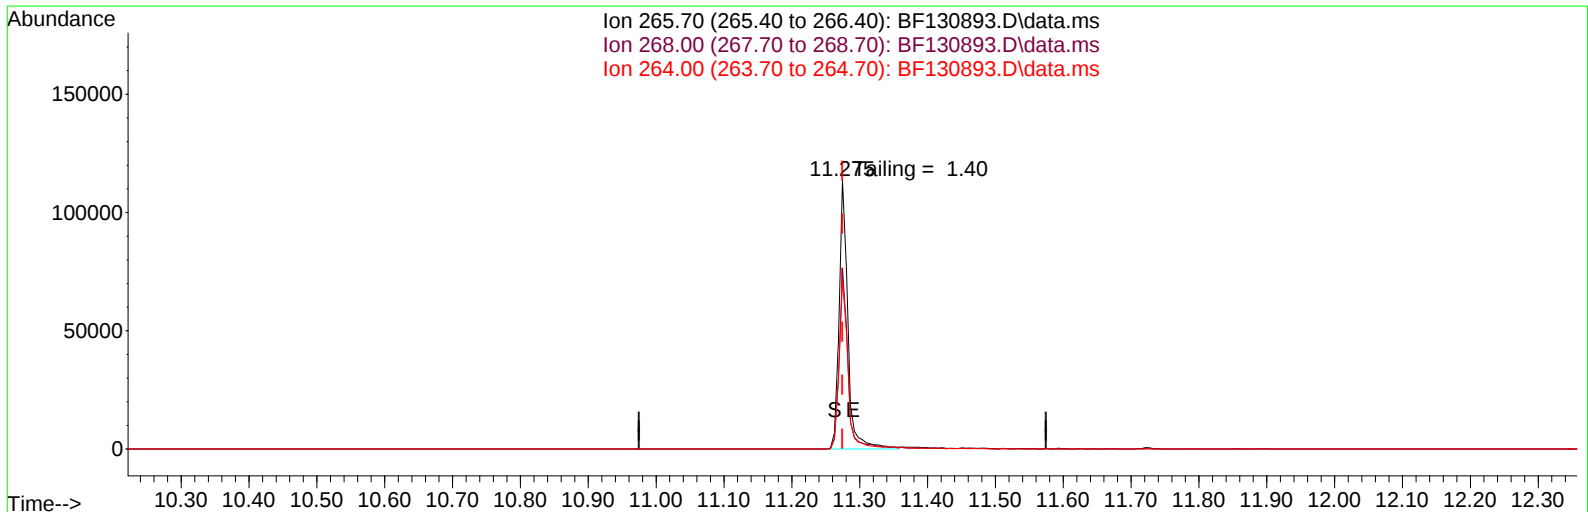

TIC: BF130893.D\data.ms

(70) Pentachlorophenol (C)

11.275min (+ 0.000) 21286.44 ng




response 102556

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.03
264.00	64.50	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
Data File : BF130893.D
Acq On : 01 Nov 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 02 10:51:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 08:18:35 2022
Response via : Initial Calibration

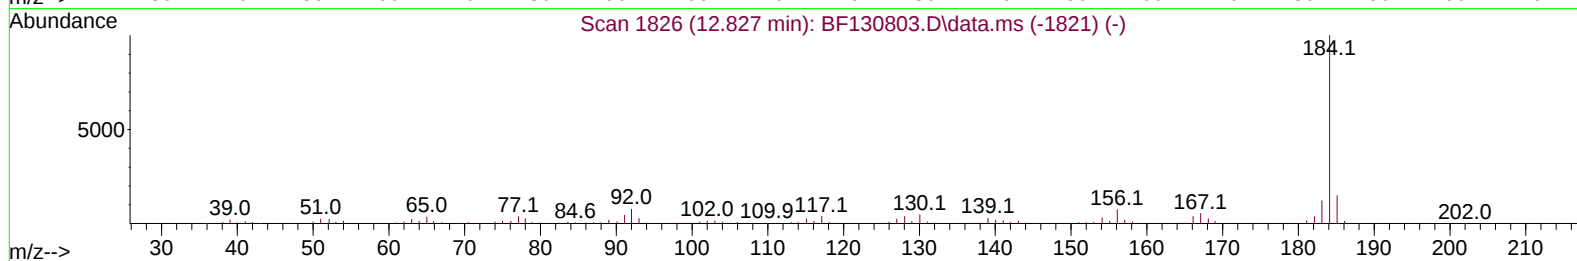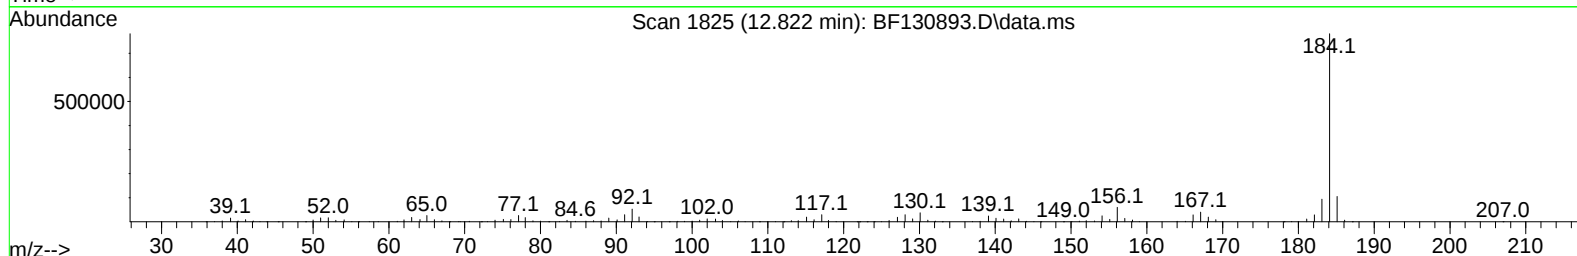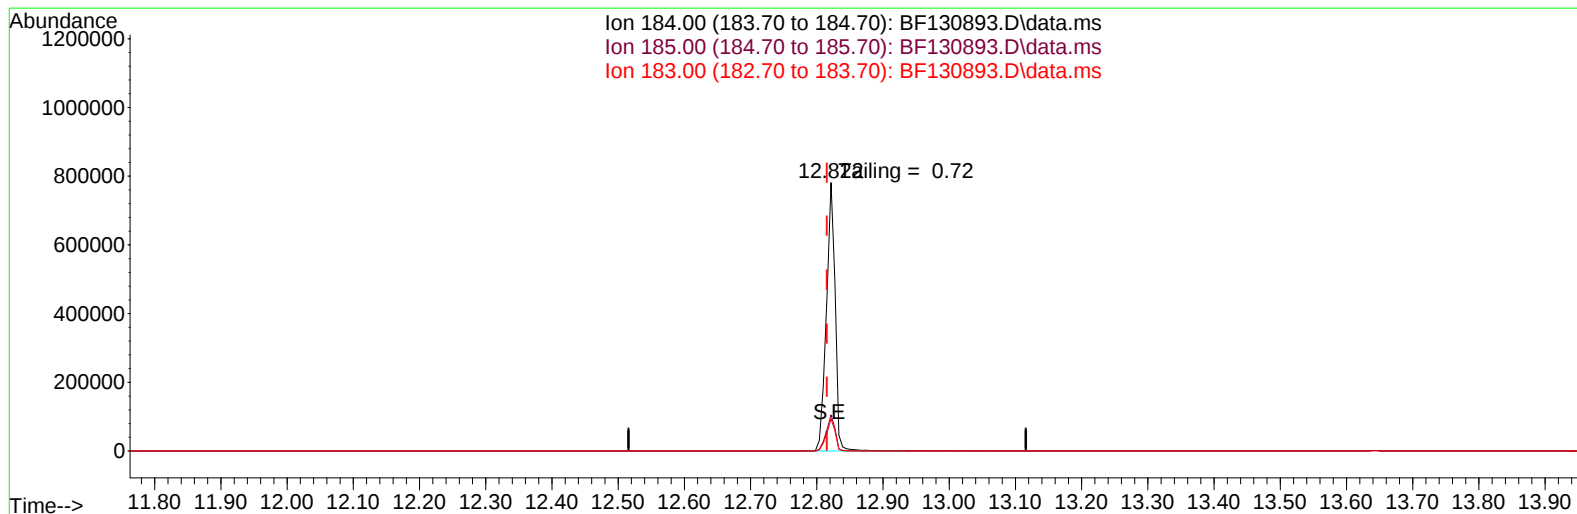

TIC: BF130893.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 392642.27 ng

response 724384

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.50
183.00	12.10	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2022	BNA_F	<u>BF130893.D</u>
Compound Name	Response	Retention Time
DDT	323041	13.645
DDD	7386	13.339
DDE	1483	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8869	331910	2.67

Instrument :
BNA_F
ClientSampleId :
DFTPP