
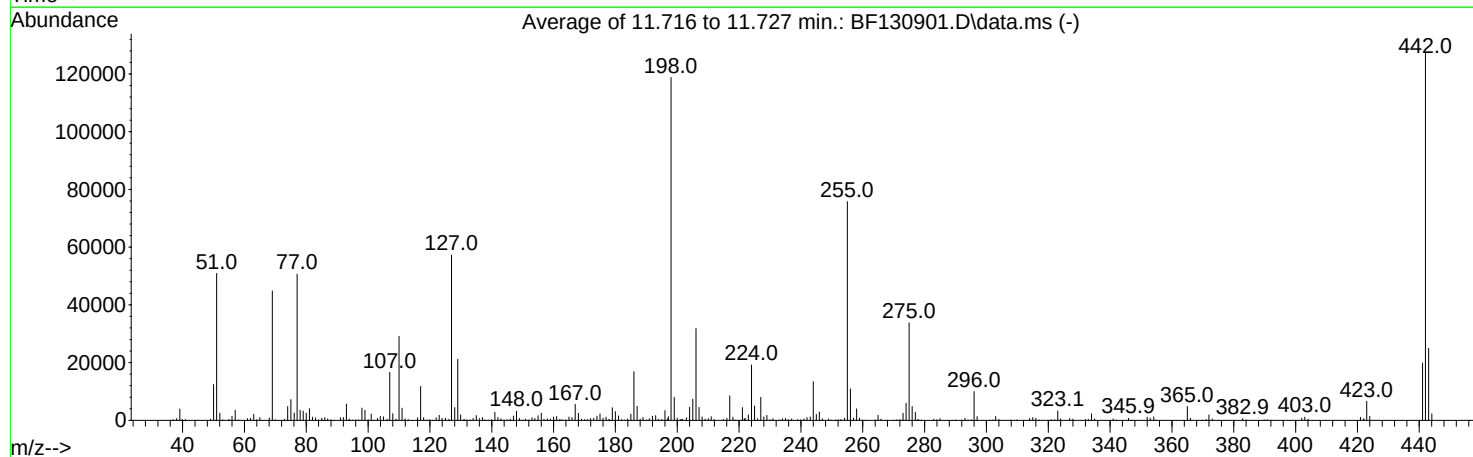


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
Data File : BF130901.D
Acq On : 01 Nov 2022 15:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 07 00:46:02 2022

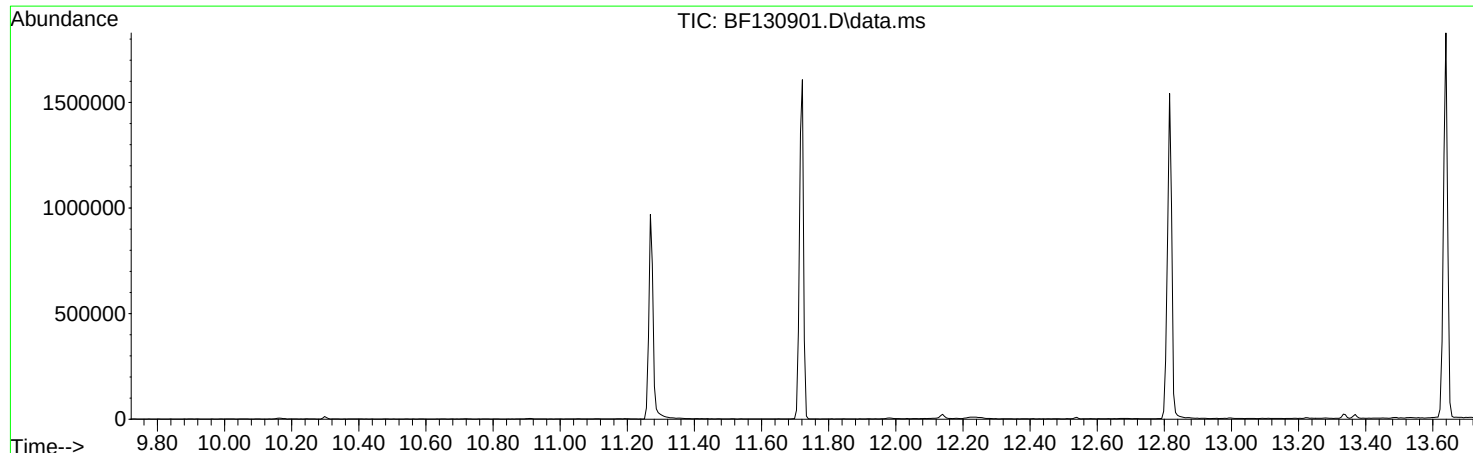




AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	50865	PASS
68	69	0.00	2	1.9	838	PASS
69	198	0.00	100	37.7	44838	PASS
70	69	0.00	2	0.3	116	PASS
127	198	10	80	48.2	57240	PASS
197	198	0.00	2	1.1	1260	PASS
198	198	100	100	100.0	118813	PASS
199	198	5	9	6.7	7966	PASS
275	198	10	60	28.4	33751	PASS
365	198	1	100	4.0	4733	PASS
441	198	0.01	100	16.7	19808	PASS
442	442	50	100	100.0	127469	PASS
443	442	15	24	19.5	24912	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
 Data File : BF130901.D
 Acq On : 01 Nov 2022 15:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 02 10:53:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 02 08:18:35 2022
 Response via : Initial Calibration

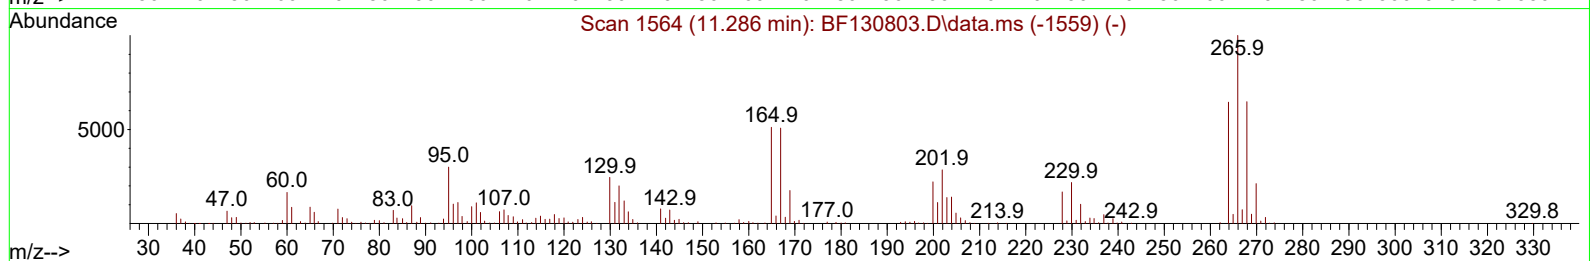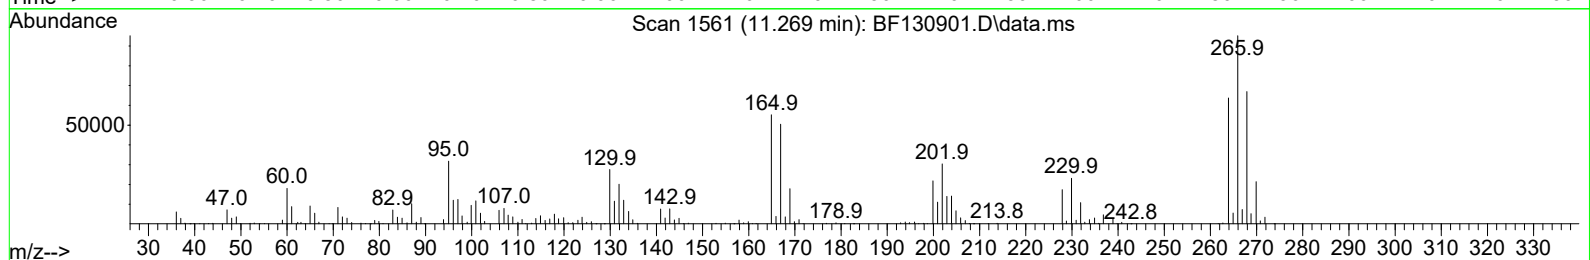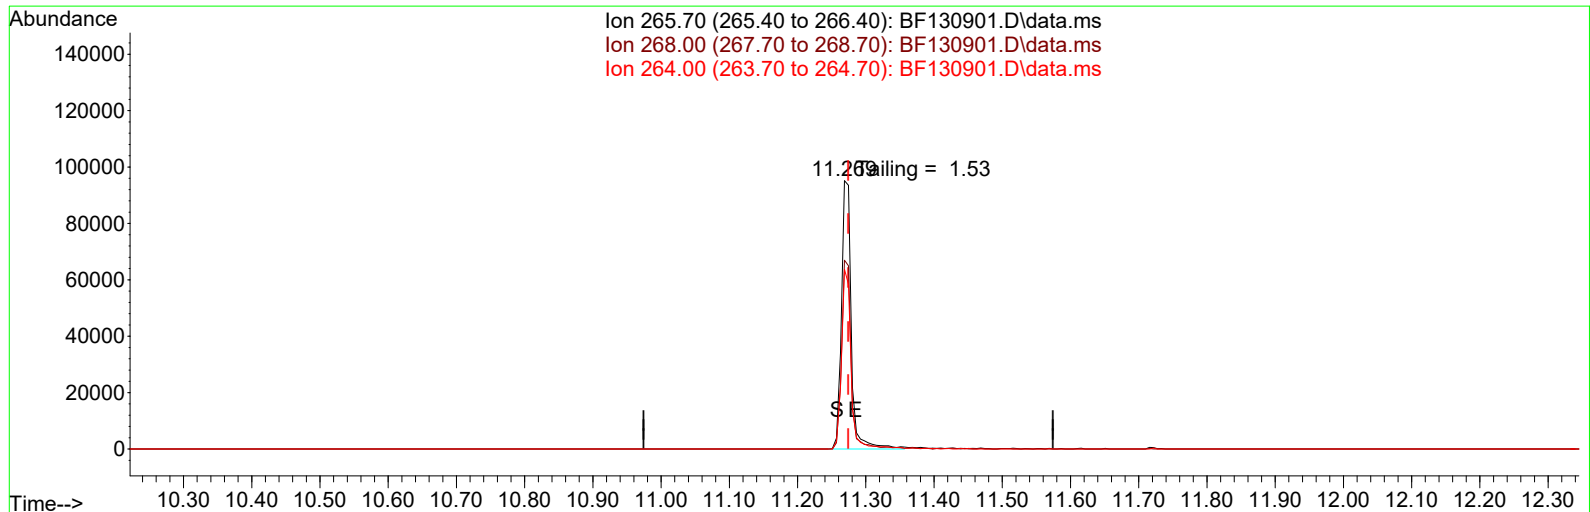

TIC: BF130901.D\data.ms

(70) Pentachlorophenol (C)

11.269min (-0.006) 29666.67 ng




response 95475

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	70.35
264.00	64.50	66.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110122\
Data File : BF130901.D
Acq On : 01 Nov 2022 15:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 02 10:53:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 08:18:35 2022
Response via : Initial Calibration

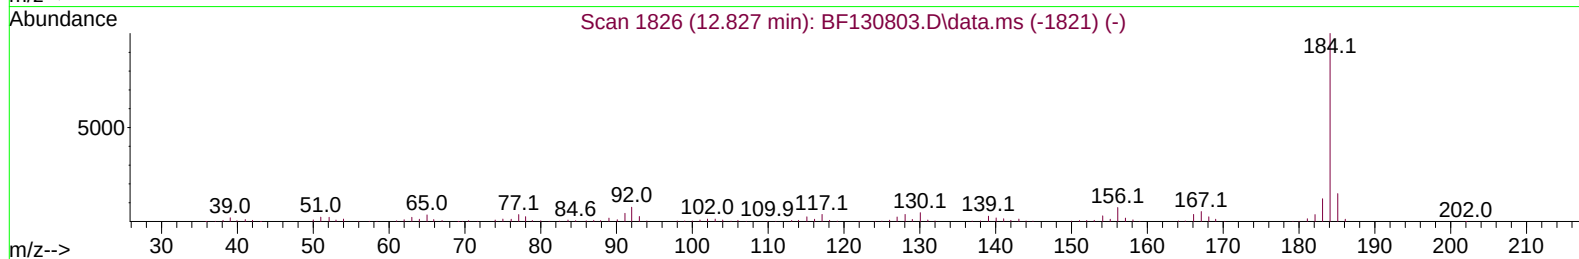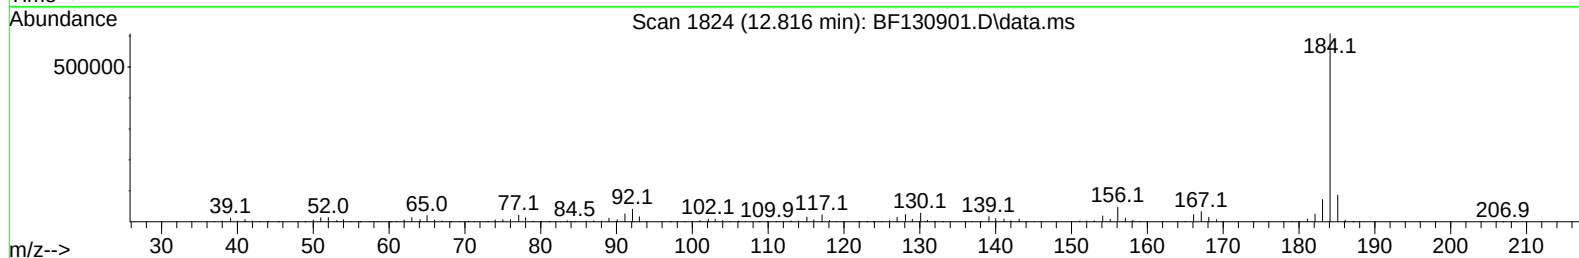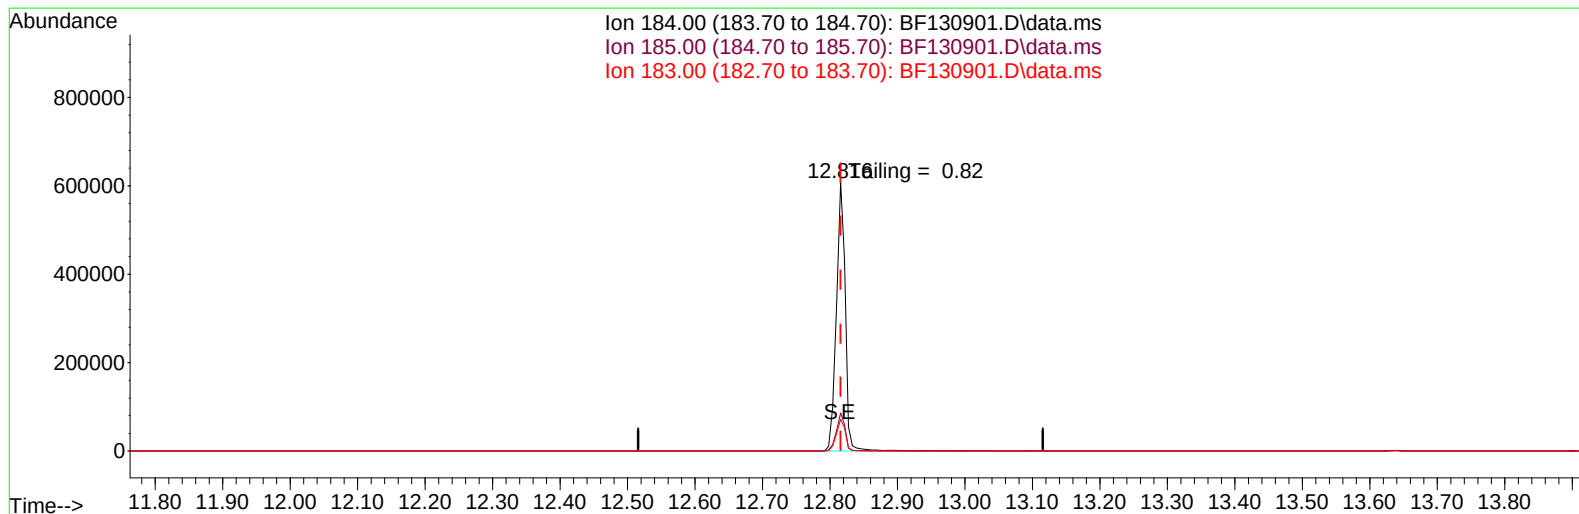

TIC: BF130901.D\data.ms

(77) Benzidine

12.816min (+ 0.000) 0.00 ng

response 558749

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.23
183.00	12.10	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2022	BNA_F	<u>BF130901.D</u>
Compound Name	Response	Retention Time
DDT	295046	13.639
DDD	6759	13.339
DDE	390	12.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7149	302195	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP