
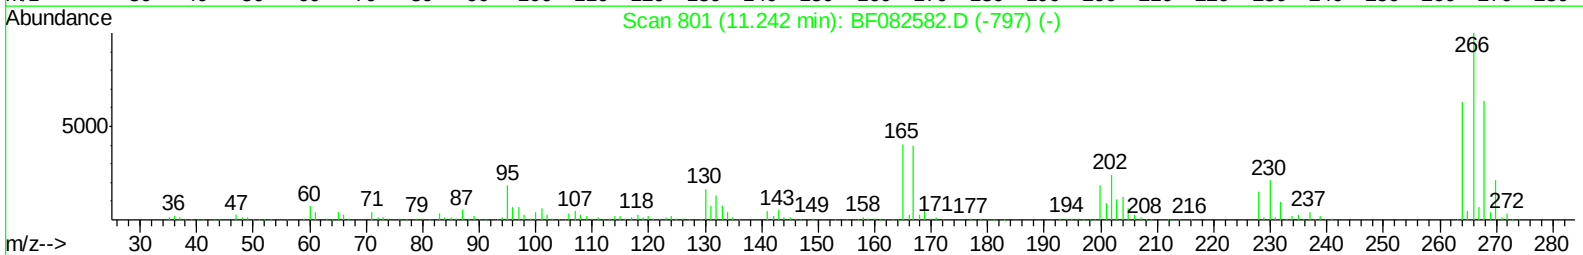
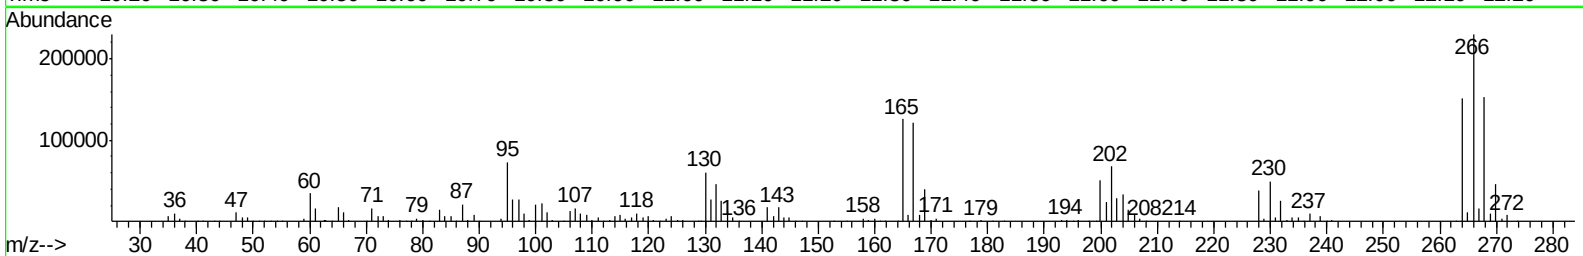


Data Path : Z:\HPCHEM1\BNA_F\Data\BF110215\
Data File : BF082633.D
Acq On : 2 Nov 2015 16:05
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:32:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

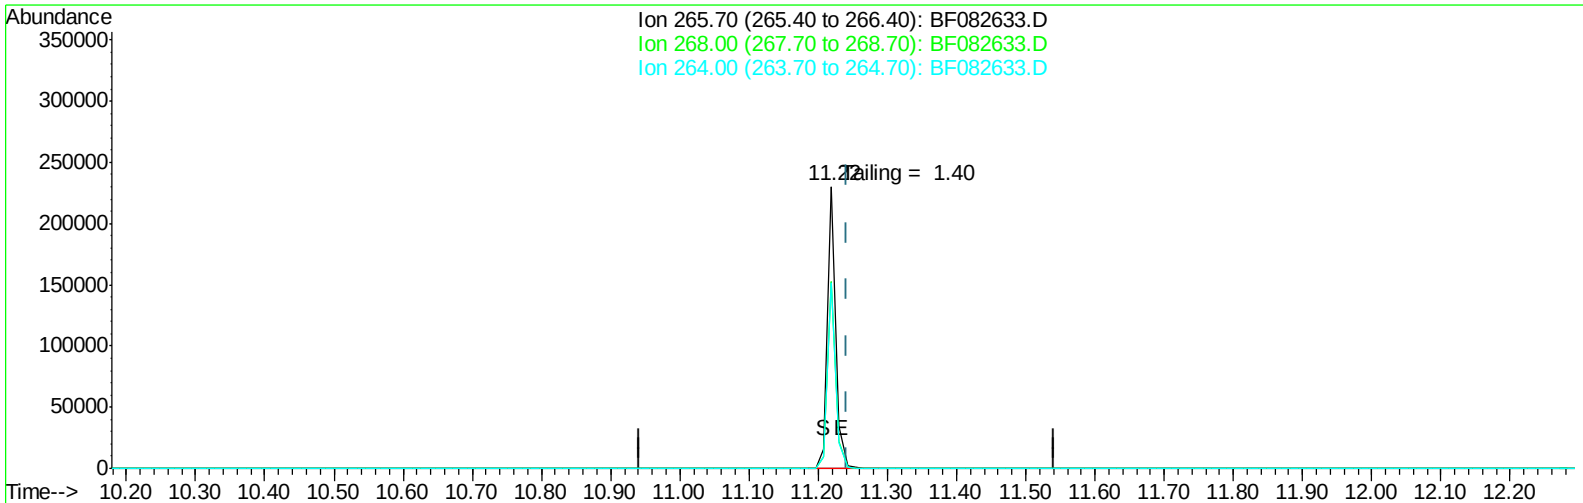

TIC: BF082633.D

(69) Pentachlorophenol (C)




11.219min (-0.023) 108254.21ng

response 194640

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	66.17
264.00	63.20	65.72
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF110215\
Data File : BF082633.D
Acq On : 2 Nov 2015 16:05
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:32:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

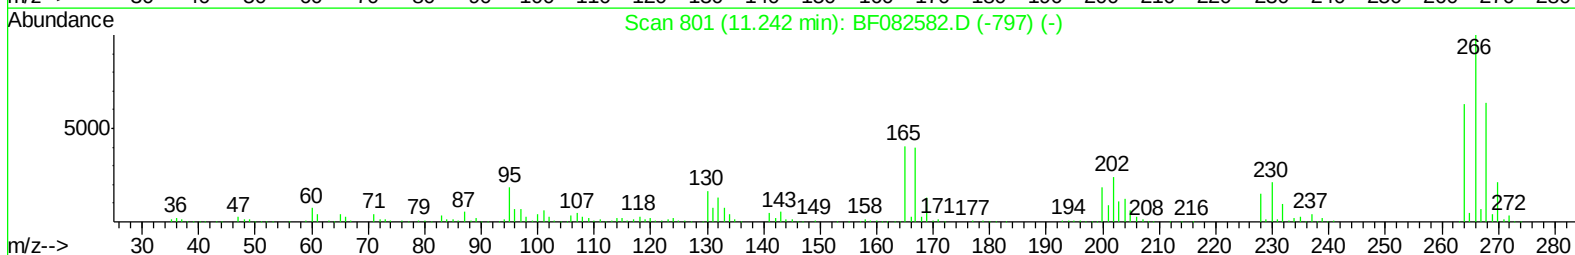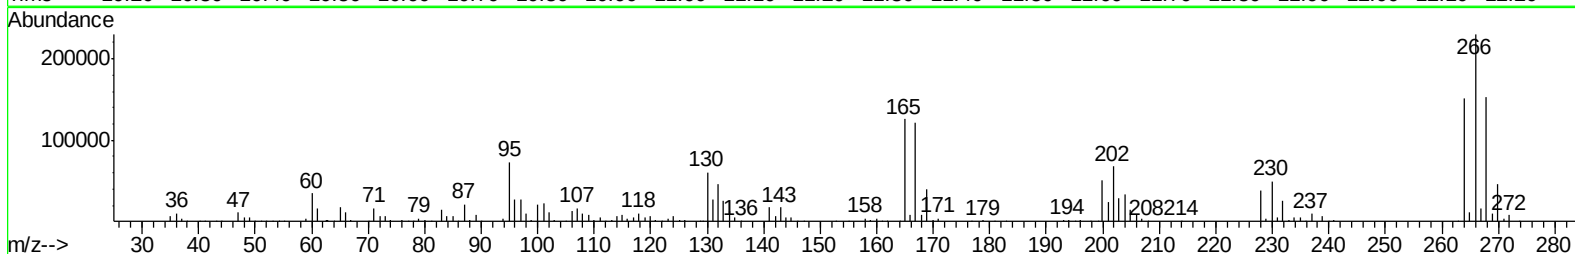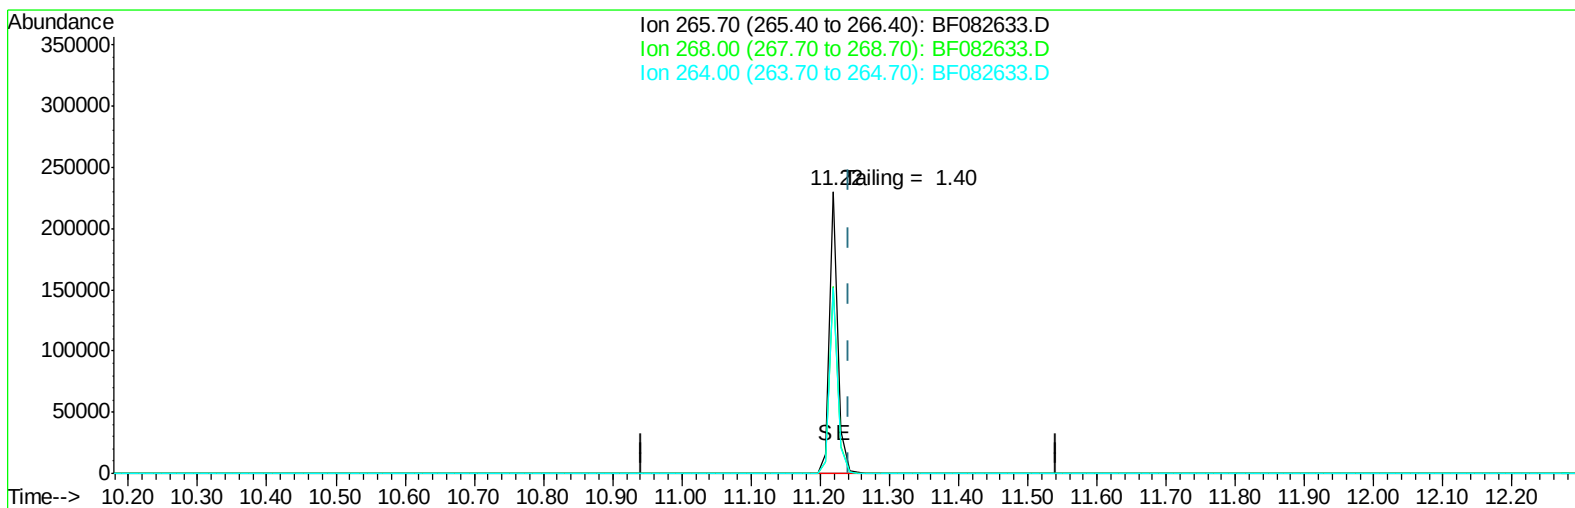

TIC: BF082633.D

(69) Pentachlorophenol (C)

11.219min (-0.023) 108254.21ng

response 194640

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	66.17
264.00	63.20	65.72
0.00	0.00	0.00