


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110215\
 Data File : BF082633.D
 Acq On : 2 Nov 2015 16:05
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 31 00:17:39 2015

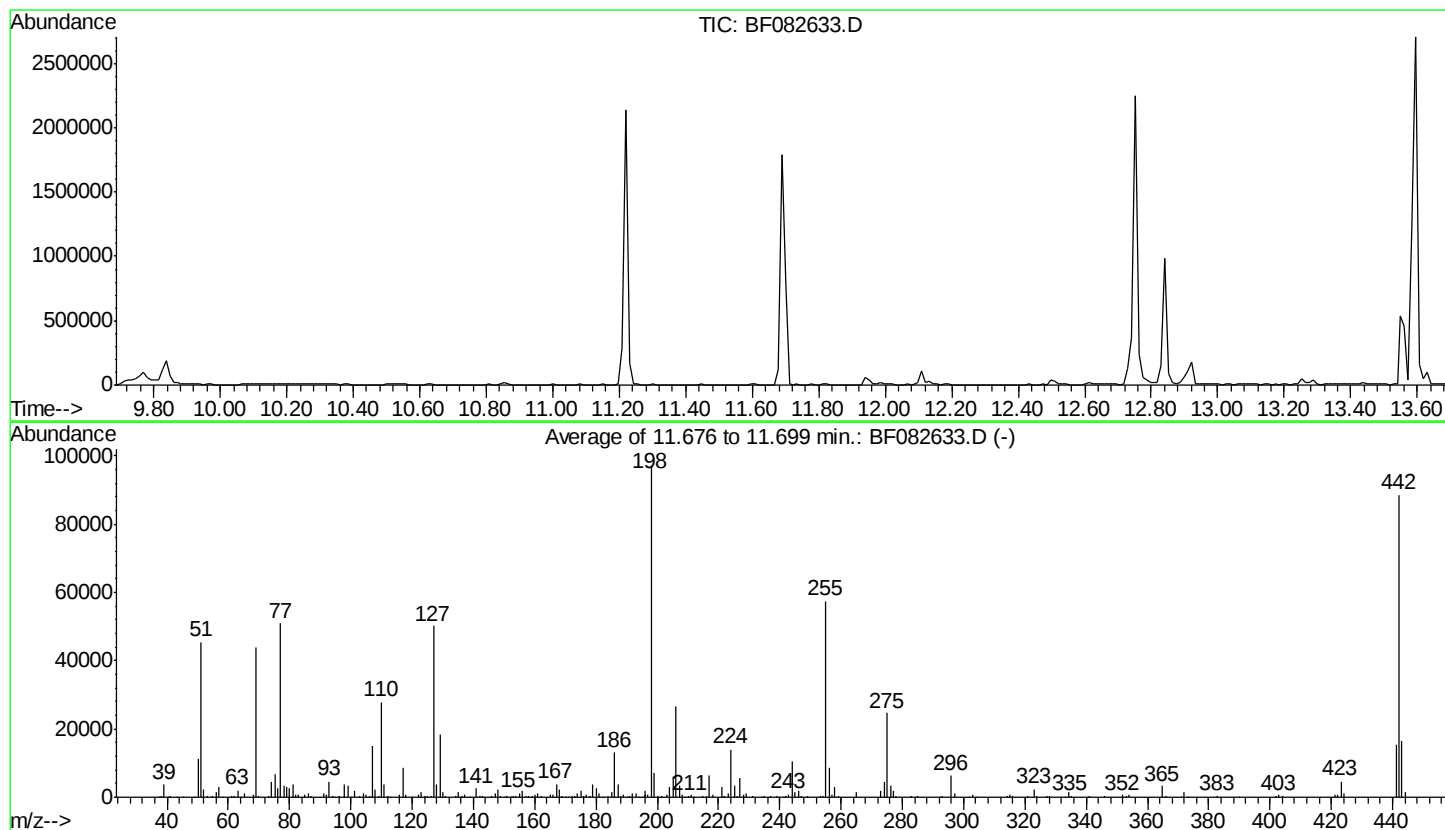

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	45585	PASS
68	69	0.00	2	1.7	761	PASS
69	198	0.00	100	45.2	43913	PASS
70	69	0.00	2	0.7	322	PASS
127	198	10	80	51.6	50146	PASS
197	198	0.00	2	0.8	769	PASS
198	198	100	100	100.0	97176	PASS
199	198	5	9	7.3	7062	PASS
275	198	10	60	25.4	24643	PASS
365	198	1	100	3.4	3295	PASS
441	442	0.01	24	17.5	15503	PASS
442	198	50	100	91.1	88543	PASS
443	442	15	24	18.8	16604	PASS