


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110216\
Data File : BF090974.D
Acq On : 2 Nov 2016 12:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 01 11:53:50 2016

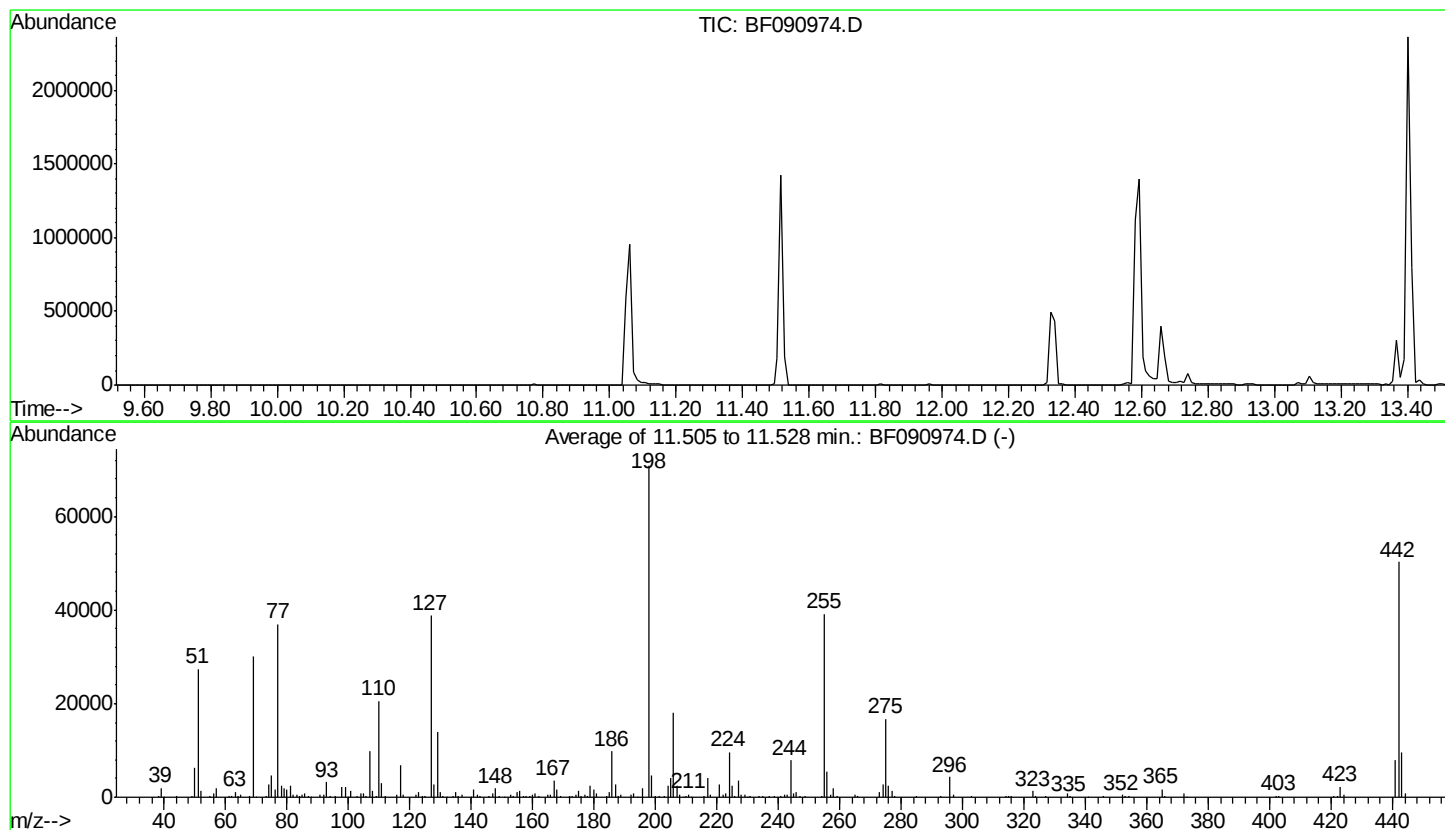

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	27439	PASS
68	69	0.00	2	1.1	334	PASS
69	198	0.00	100	42.5	30070	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	54.8	38811	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70820	PASS
199	198	5	9	6.7	4729	PASS
275	198	10	60	23.7	16752	PASS
365	198	1	100	2.4	1725	PASS
441	442	0.01	24	15.6	7863	PASS
442	198	50	100	71.0	50250	PASS
443	442	15	24	18.9	9499	PASS