
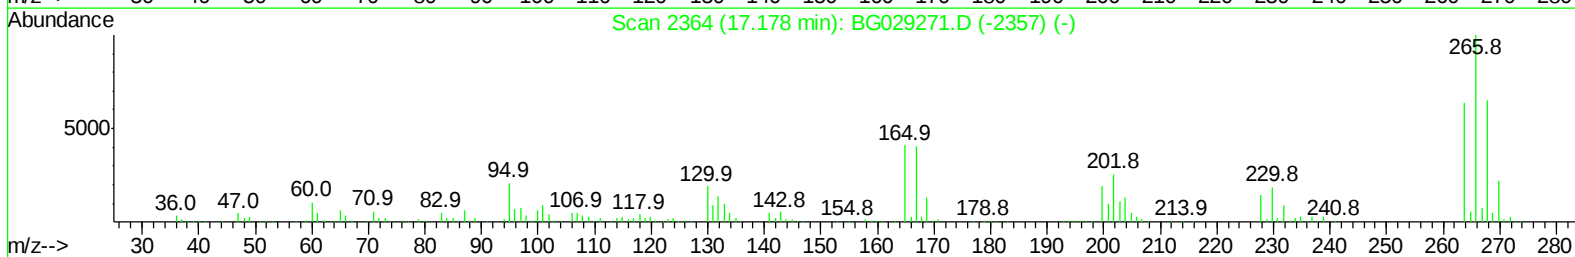
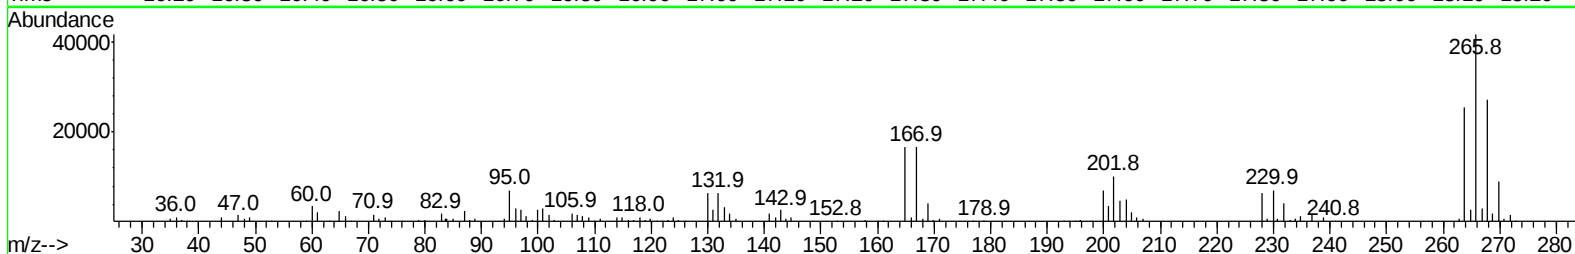


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
Data File : BG030655.D
Acq On : 2 Nov 2017 9:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 03 09:14:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

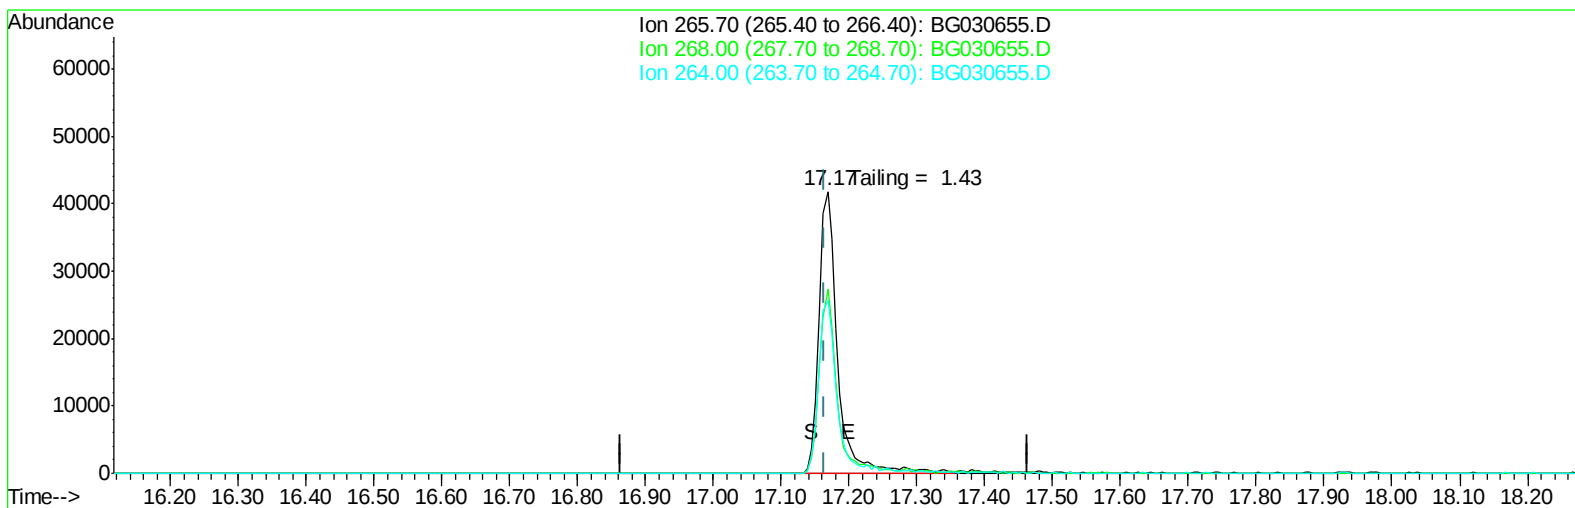

TIC: BG030655.D

(69) Pentachlorophenol (C)

17.168min (+0.003) 59038.77ng




response 76262

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.53
264.00	62.00	61.43
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
Data File : BG030655.D
Acq On : 2 Nov 2017 9:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 03 09:14:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

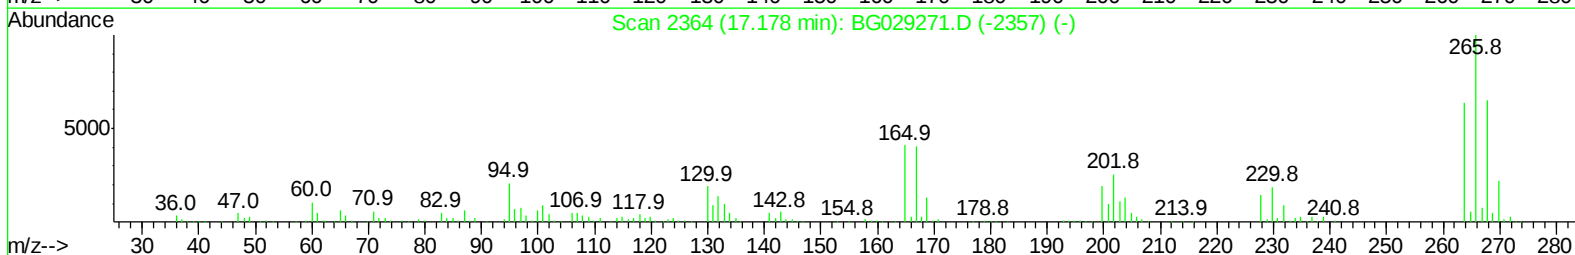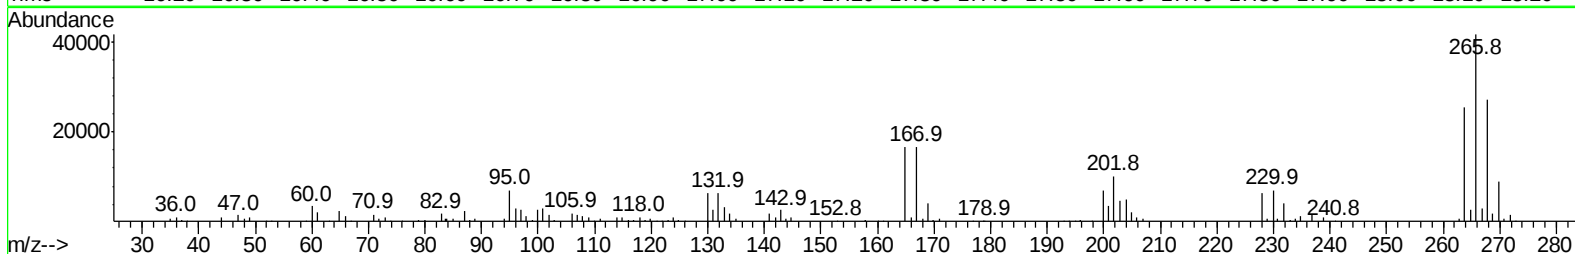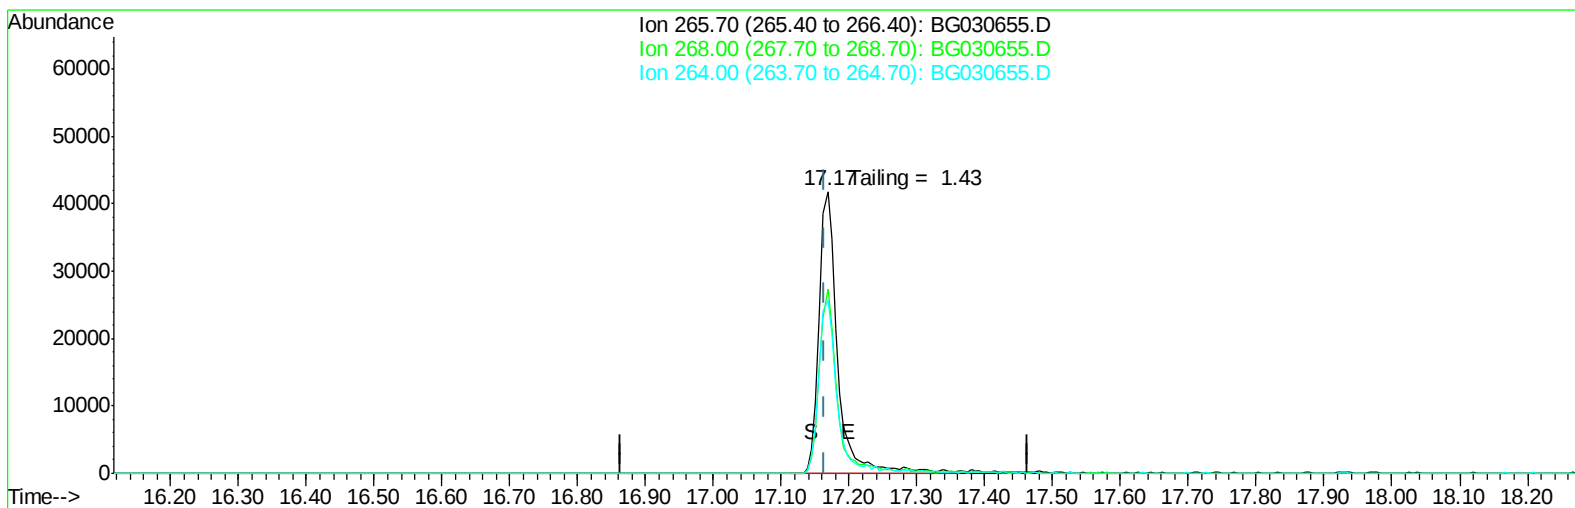

TIC: BG030655.D

(69) Pentachlorophenol (C)

17.168min (+0.003) 59038.77ng

response 76262

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.53
264.00	62.00	61.43
0.00	0.00	0.00