

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
 Data File : BF100087.D
 Acq On : 2 Nov 2017 16:19
 Operator : SJ/JU
 Sample : I6233-01 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1(3-5)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	489	492	503	rBV2	14916	27398	3.87%	0.477%
2	5.398	560	563	586	rBV	112490	234536	33.09%	4.083%
3	6.422	735	737	755	rBV	143713	255881	36.10%	4.455%
4	6.545	755	758	769	rVB	277765	306778	43.28%	5.341%
5	6.769	793	796	808	rBV	490557	464038	65.47%	8.078%
6	6.922	819	822	838	rBV	221590	235364	33.21%	4.097%
7	7.345	891	894	912	rBV	107109	155804	21.98%	2.712%
8	8.051	1011	1014	1024	rBV	745045	638950	90.15%	11.123%
9	9.122	1193	1196	1206	rVB	427955	381029	53.76%	6.633%
10	9.527	1262	1265	1272	rBV	51888	44226	6.24%	0.770%
11	9.810	1309	1313	1320	rBV	766667	708776	100.00%	12.339%
12	10.222	1381	1383	1387	rVB	12738	9416	1.33%	0.164%
13	10.527	1431	1435	1440	rBB	18329	17420	2.46%	0.303%
14	10.604	1445	1448	1459	rVB	170720	173568	24.49%	3.022%
15	11.304	1563	1567	1576	rBV	697605	665398	93.88%	11.584%
16	11.645	1621	1625	1628	rBV2	8765	10891	1.54%	0.190%
17	11.851	1656	1660	1667	rVB	8107	12123	1.71%	0.211%
18	12.527	1772	1775	1780	rBV	10096	10750	1.52%	0.187%
19	12.763	1813	1815	1821	rVB	13994	12544	1.77%	0.218%
20	12.880	1832	1835	1840	rVB	320299	303497	42.82%	5.284%
21	13.445	1928	1931	1935	rBV3	6234	8228	1.16%	0.143%
22	13.786	1987	1989	1994	rVB6	12863	14550	2.05%	0.253%
23	13.933	2008	2014	2017	rBV	23773	33993	4.80%	0.592%
24	13.980	2019	2022	2030	rVV	446379	478437	67.50%	8.329%
25	14.457	2099	2103	2105	rBV4	8121	10459	1.48%	0.182%
26	14.780	2156	2158	2162	rBV4	12653	15095	2.13%	0.263%
27	15.027	2198	2200	2202	rBV3	10351	11659	1.64%	0.203%
28	15.092	2209	2211	2212	rBV2	14195	11451	1.62%	0.199%
29	15.515	2279	2283	2292	rVB	354320	463993	65.46%	8.078%
30	15.598	2294	2297	2301	rVB6	12573	15982	2.25%	0.278%
31	16.398	2431	2433	2434	rBV2	16517	11918	1.68%	0.207%


Sum of corrected areas: 5744152

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110217\
Data File : BF100087.D
Acq On : 2 Nov 2017 16:19
Operator : SJ/JU
Sample : I6233-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1(3-5)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

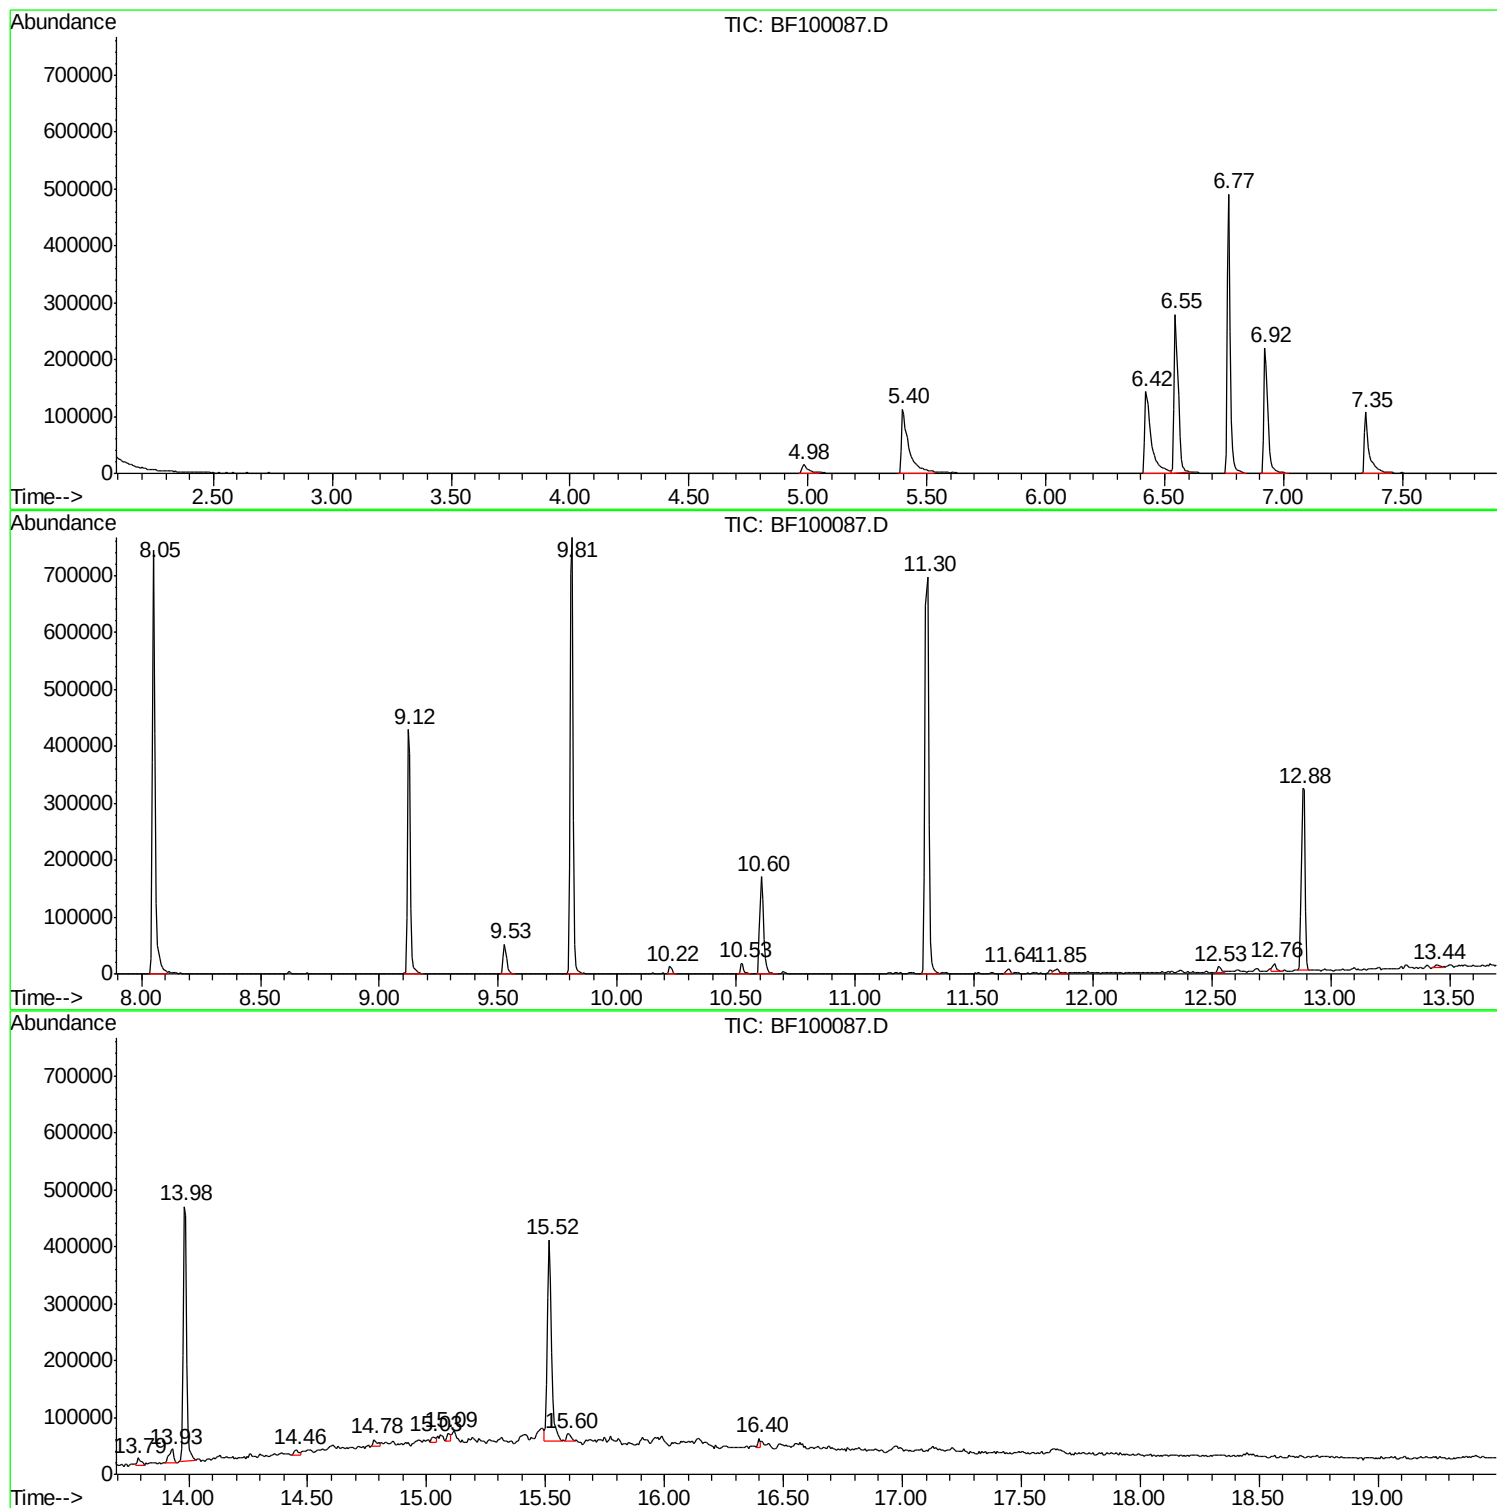

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110217\
Data File : BF100087.D
Acq On : 2 Nov 2017 16:19
Operator : SJ/JU
Sample : I6233-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1(3-5)










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.55	13.22 ng	306778	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	9

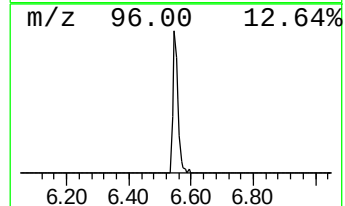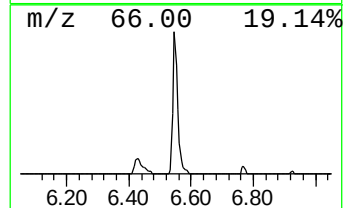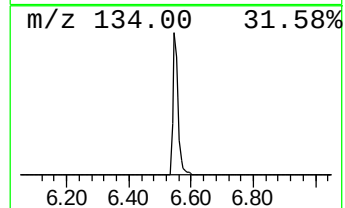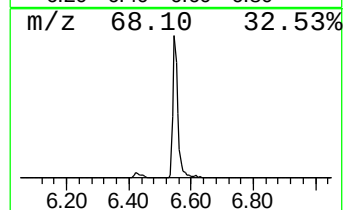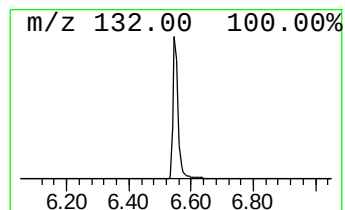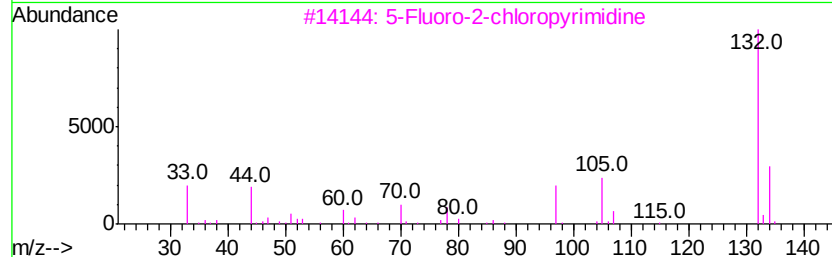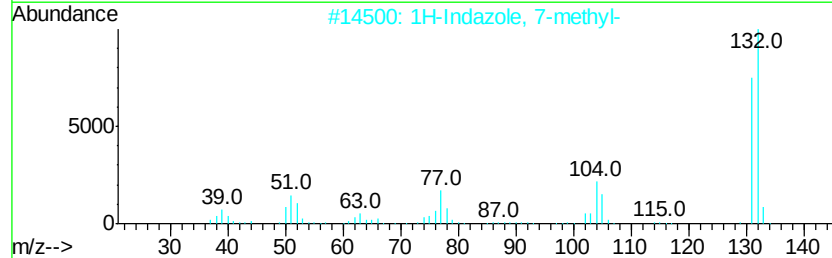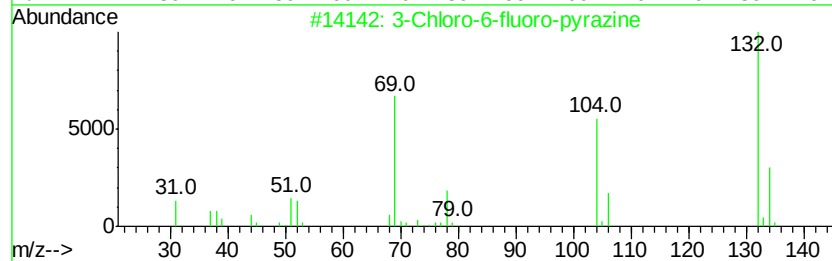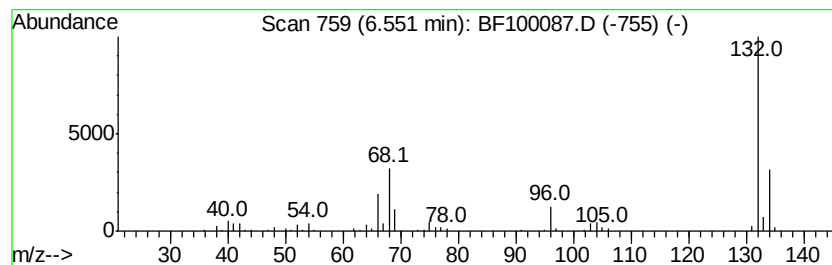

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
Data File : BF100087.D
Acq On : 2 Nov 2017 16:19
Operator : SJ/JU
Sample : I6233-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1(3-5)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.55	6.55	13.2	ng	306778	1	6.77	464038	20.0