

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
 Data File : BF100116.D
 Acq On : 3 Nov 2017 6:21
 Operator : SJ/JU
 Sample : I6273-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 103117-TIDO-E-D-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	489	492	510	rBV	109702	156598	5.64%	0.781%
2	5.398	560	563	587	rBV	535657	824233	29.70%	4.113%
3	6.416	734	736	754	rBV	415167	584079	21.05%	2.915%
4	6.539	754	757	769	rVB	1443507	1479614	53.32%	7.384%
5	6.769	793	796	805	rBV	534544	482167	17.38%	2.406%
6	6.922	818	822	834	rBV	1992385	1947600	70.18%	9.719%
7	7.345	889	894	911	rBV	1451903	1498417	54.00%	7.477%
8	8.051	1010	1014	1016	rBV	812038	742134	26.74%	3.703%
9	8.069	1016	1017	1025	rVB	704771	618604	22.29%	3.087%
10	8.763	1132	1135	1143	rBV	197984	179608	6.47%	0.896%
11	8.863	1149	1152	1160	rVB	115775	106370	3.83%	0.531%
12	9.127	1192	1197	1200	rBV	3008201	2775005	100.00%	13.848%
13	9.227	1211	1214	1220	rVB	64810	57540	2.07%	0.287%
14	9.804	1309	1312	1315	rVB2	859642	703013	25.33%	3.508%
15	9.833	1315	1317	1326	rVB	295492	279578	10.07%	1.395%
16	10.016	1344	1348	1353	rBV	175955	176296	6.35%	0.880%
17	10.357	1403	1406	1412	rBV	204772	180045	6.49%	0.898%
18	10.474	1423	1426	1430	rBV	106982	87854	3.17%	0.438%
19	10.516	1430	1433	1439	rVB2	37994	41245	1.49%	0.206%
20	10.604	1444	1448	1461	rVB	1028378	1063307	38.32%	5.306%
21	11.298	1562	1566	1568	rBV	805947	716139	25.81%	3.574%
22	11.321	1568	1570	1574	rVB	486406	378653	13.65%	1.890%
23	11.545	1605	1608	1613	rBV	41017	43312	1.56%	0.216%
24	11.810	1649	1653	1655	rBV2	58570	57949	2.09%	0.289%
25	11.833	1655	1657	1663	rVB2	23930	35955	1.30%	0.179%
26	11.916	1668	1671	1673	rBV	37823	33716	1.21%	0.168%
27	12.321	1737	1740	1744	rBV	35039	34098	1.23%	0.170%
28	12.515	1768	1773	1780	rBV	155290	147000	5.30%	0.734%
29	12.598	1784	1787	1795	rBV2	22291	32289	1.16%	0.161%
30	12.733	1805	1810	1811	rBV	55380	50448	1.82%	0.252%
31	12.751	1811	1813	1818	rVB	79987	75447	2.72%	0.377%
32	12.880	1830	1835	1838	rBV	2271825	2415611	87.05%	12.055%
33	13.086	1864	1870	1874	rBV2	90673	104089	3.75%	0.519%
34	13.427	1925	1928	1932	rVB	91507	83579	3.01%	0.417%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
Data File : BF100116.D
Acq On : 3 Nov 2017 6:21
Operator : SJ/JU
Sample : I6273-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
103117-TIDO-E-D-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.757	1980	1984	1991	rBV	72615	78527	2.83%	0.392%
36	13.951	2013	2017	2023	rBV	494490	531837	19.17%	2.654%
37	14.074	2030	2038	2040	rBV5	49219	122323	4.41%	0.610%
38	14.457	2098	2103	2111	rVB9	13769	31980	1.15%	0.160%
39	15.021	2189	2199	2216	rVB4	122952	428699	15.45%	2.139%
40	15.404	2260	2264	2276	rVB	318033	417931	15.06%	2.086%
41	16.968	2516	2530	2536	rBV5	52635	236148	8.51%	1.178%


Sum of corrected areas: 20039037

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110217\
Data File : BF100116.D
Acq On : 3 Nov 2017 6:21
Operator : SJ/JU
Sample : I6273-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
103117-TIDO-E-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

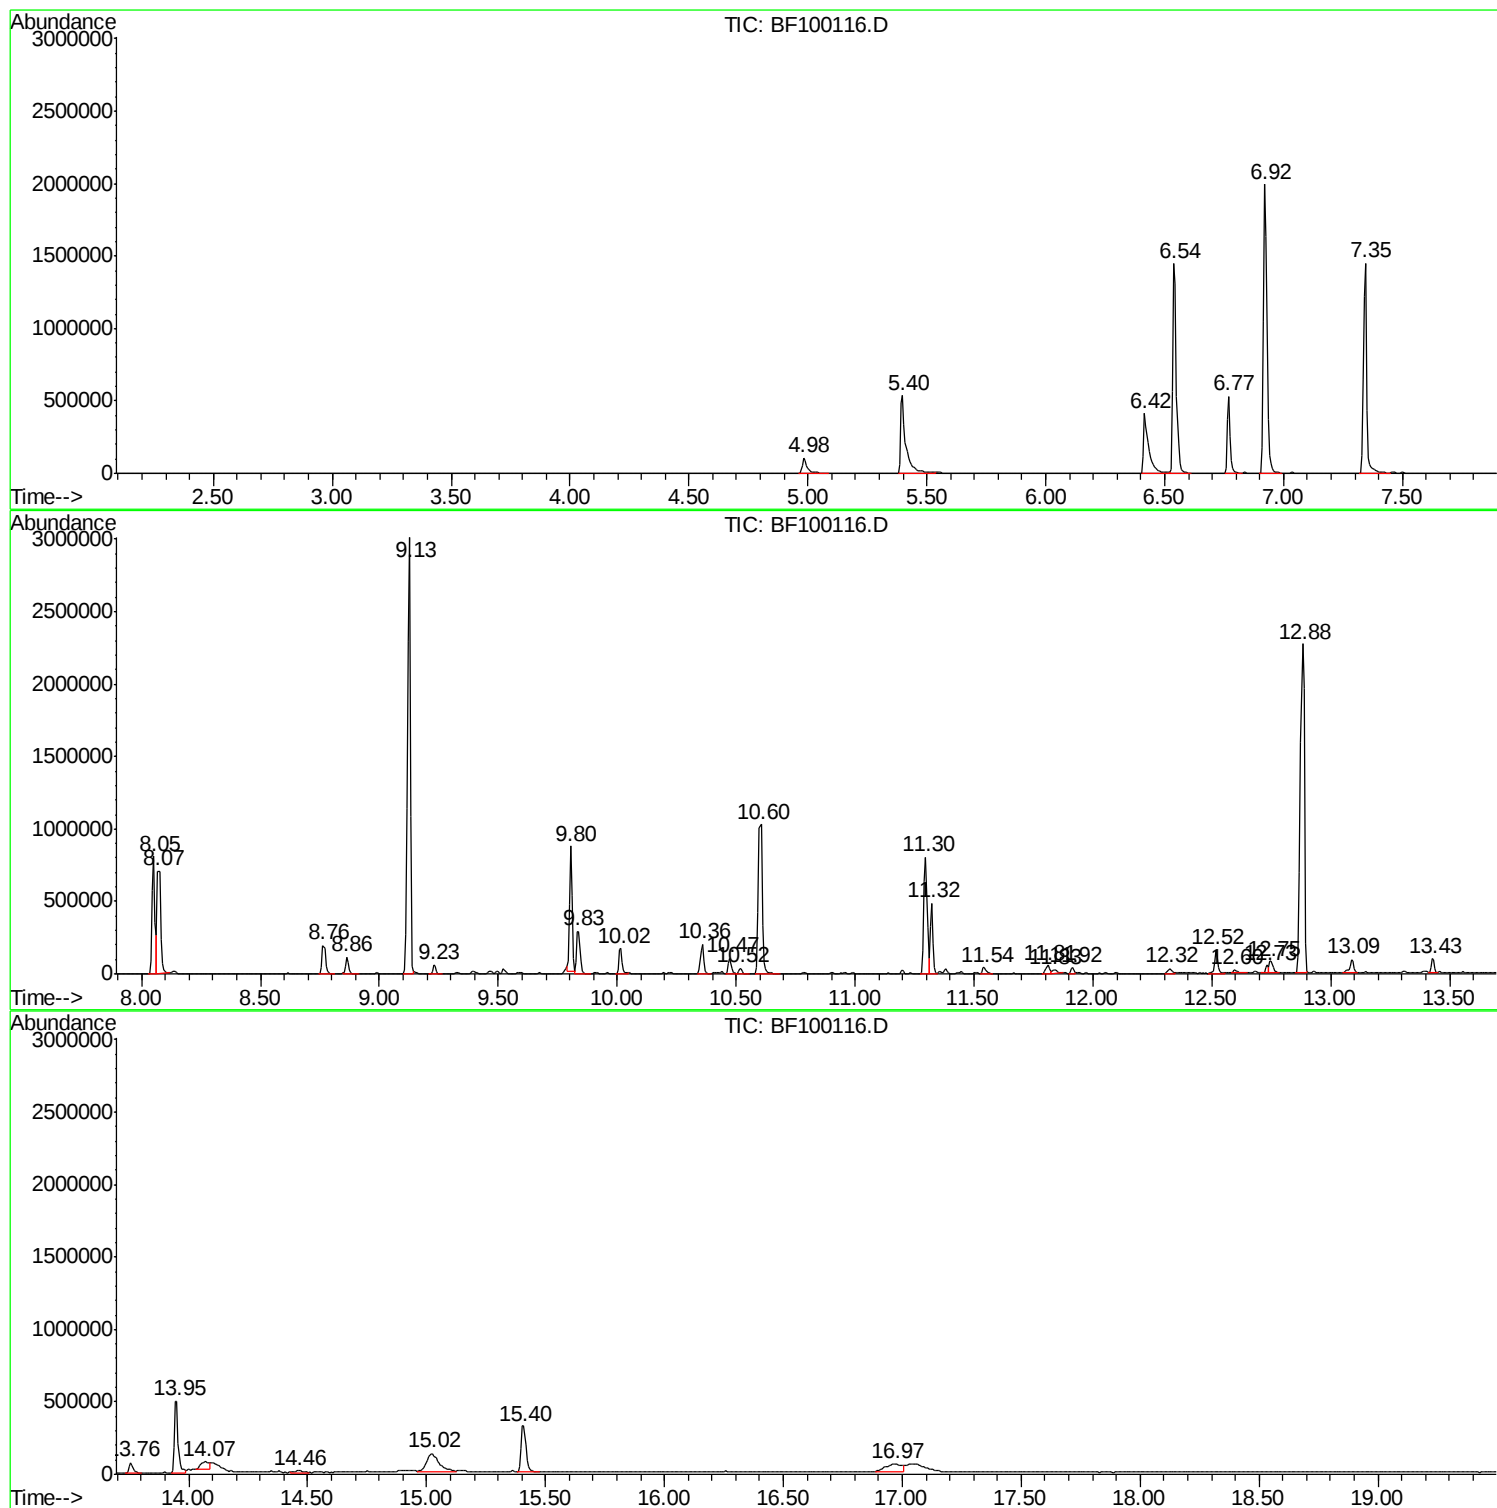

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
Data_File : BF100116.D
Acq_On : 3-Nov-2017 6:211
Operator : SJ/JUU
Sample : I6273-011
Misc :
ALS_Vial : 35 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
103117-TIDO-E-D-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
