

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
 Data File : BF100117.D
 Acq On : 3 Nov 2017 6:48
 Operator : SJ/JU
 Sample : I6273-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 103117-TIDO-E-D-S

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	489	492	510	rBV	92952	130916	5.29%	0.861%
2	5.398	560	563	589	rBV	391216	666427	26.92%	4.384%
3	6.422	734	737	754	rBV	262493	433333	17.51%	2.850%
4	6.540	754	757	771	rVB	1241326	1254918	50.70%	8.254%
5	6.769	793	796	805	rBV	476009	440357	17.79%	2.897%
6	6.922	818	822	839	rBV	1829075	1704409	68.86%	11.211%
7	7.340	889	893	912	rBV	1223235	1266891	51.18%	8.333%
8	8.051	1010	1014	1016	rBV	697255	592528	23.94%	3.897%
9	8.075	1016	1018	1027	rVB	116115	127809	5.16%	0.841%
10	8.769	1134	1136	1144	rBB	33169	31501	1.27%	0.207%
11	9.128	1192	1197	1200	rBV	2461579	2475146	100.00%	16.281%
12	9.804	1304	1312	1316	rBV	802924	712792	28.80%	4.688%
13	9.839	1316	1318	1323	rVB	61889	53216	2.15%	0.350%
14	10.016	1346	1348	1358	rBB	27931	29927	1.21%	0.197%
15	10.357	1404	1406	1413	rVB	36987	35269	1.42%	0.232%
16	10.475	1423	1426	1431	rBB	68396	55429	2.24%	0.365%
17	10.598	1444	1447	1460	rBV	909044	893935	36.12%	5.880%
18	11.298	1562	1566	1568	rBV	726393	644941	26.06%	4.242%
19	11.322	1568	1570	1575	rVB	95662	87178	3.52%	0.573%
20	12.522	1768	1774	1778	rBV	33689	32601	1.32%	0.214%
21	12.680	1798	1801	1807	rBV	59996	47764	1.93%	0.314%
22	12.757	1811	1814	1819	rVB2	27097	31077	1.26%	0.204%
23	12.880	1830	1835	1838	rBV	2170799	2074952	83.83%	13.648%
24	13.086	1864	1870	1873	rBV	36916	32160	1.30%	0.212%
25	13.386	1918	1921	1924	rVB	37659	30628	1.24%	0.201%
26	13.757	1981	1984	1990	rBV	23634	26465	1.07%	0.174%
27	13.945	2013	2016	2024	rBV	472071	460189	18.59%	3.027%
28	14.951	2170	2187	2188	rBV6	46796	164510	6.65%	1.082%
29	15.004	2191	2196	2211	rVB4	77178	292464	11.82%	1.924%
30	15.410	2260	2265	2275	rVB	290181	373337	15.08%	2.456%


Sum of corrected areas: 15203069

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110217\
Data File : BF100117.D
Acq On : 3 Nov 2017 6:48
Operator : SJ/JU
Sample : I6273-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
103117-TIDO-E-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

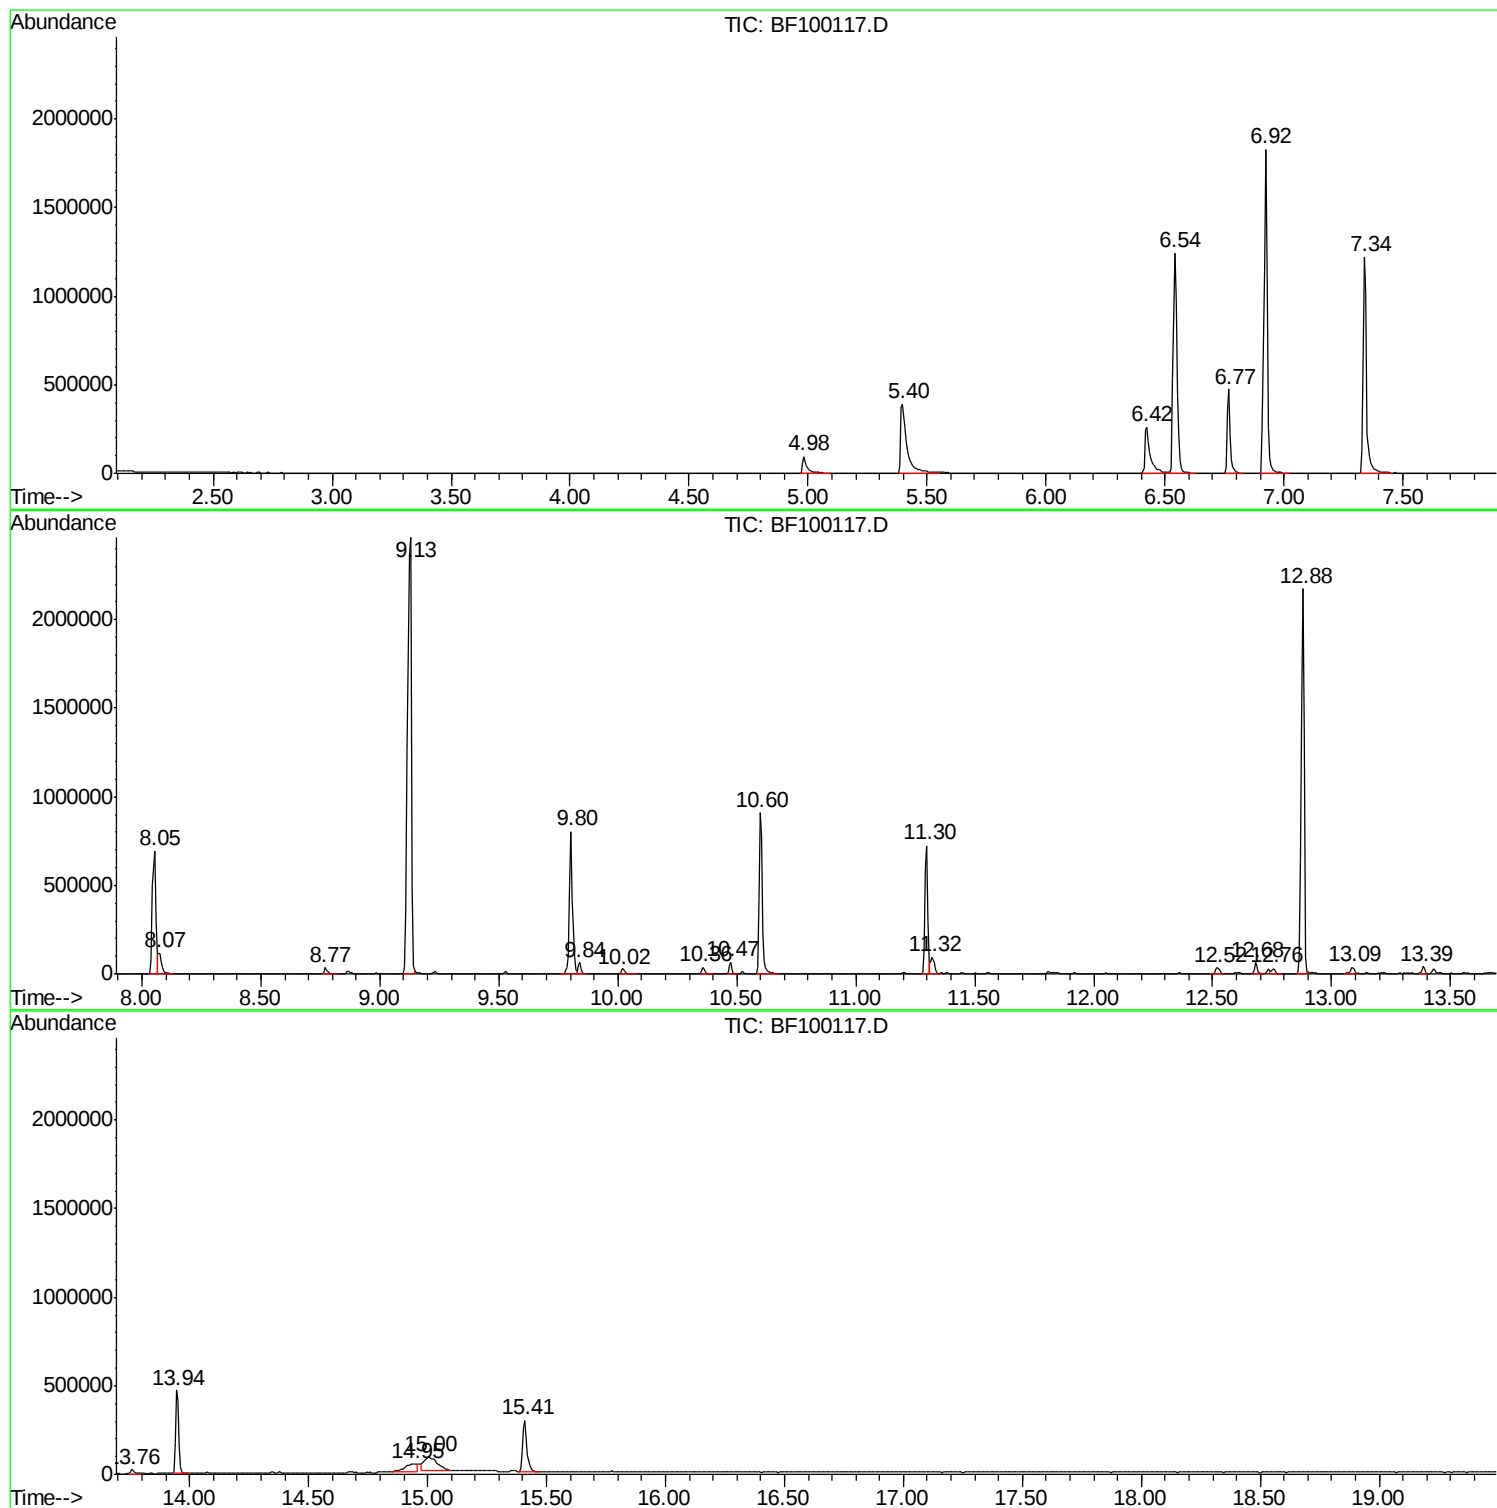

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110217\
Data_File : BF100117.D
Acq_On : 3-Nov-2017 6:488
Operator : SJ/JUU
Sample : I6273-022
Misc :
ALS_Vial : 36 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
103117-TIDO-E-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
