
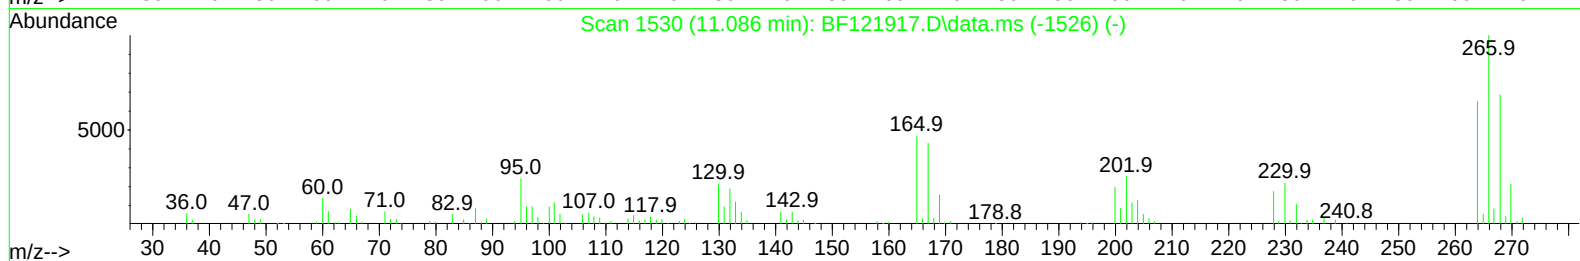
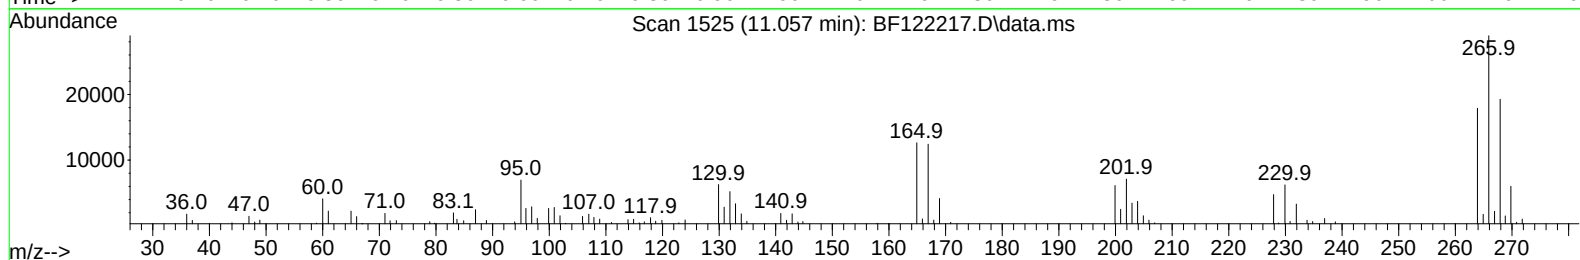


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110220\
Data File : BF122217.D
Acq On : 2 Nov 2020 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 01:09:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

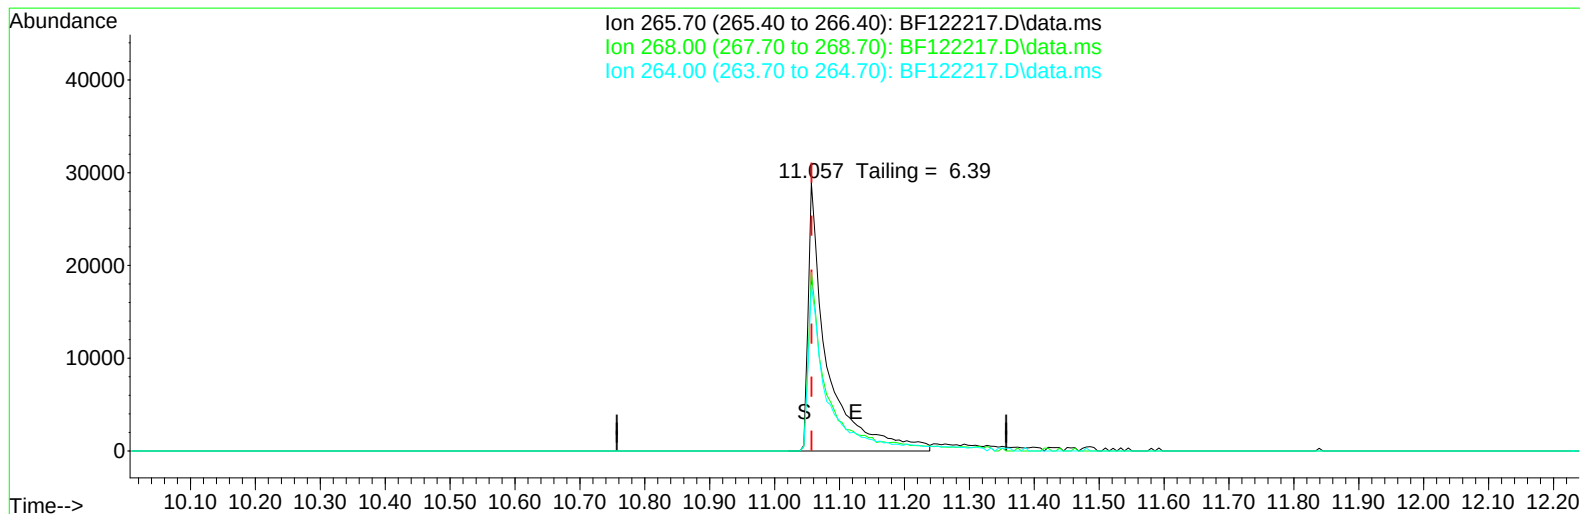

TIC: BF122217.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.000) 91598.59 ng

response 58558

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	66.62
264.00	62.40	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110220\
Data File : BF122217.D
Acq On : 2 Nov 2020 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 01:09:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

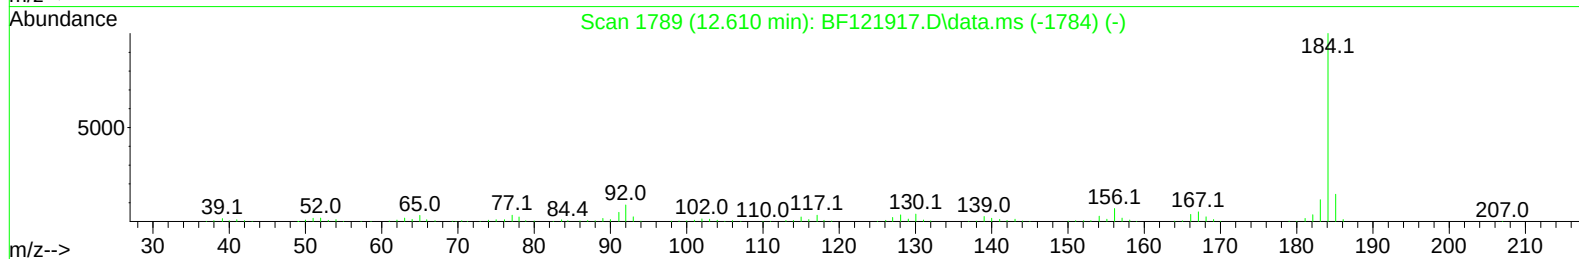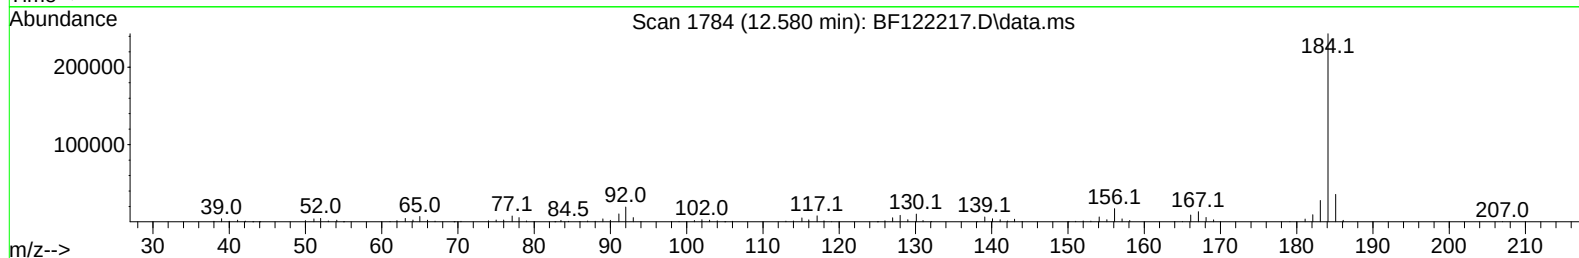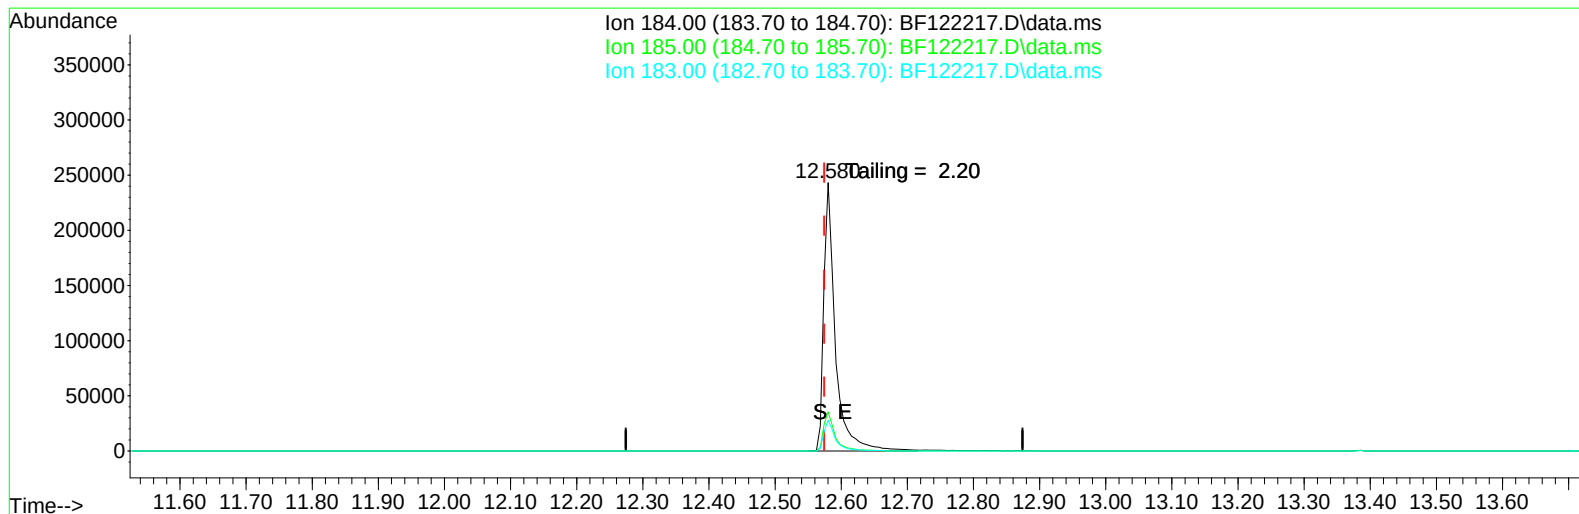

TIC: BF122217.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 0.00 ng

response 295974

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.64
183.00	11.70	11.46
0.00	0.00	0.00