
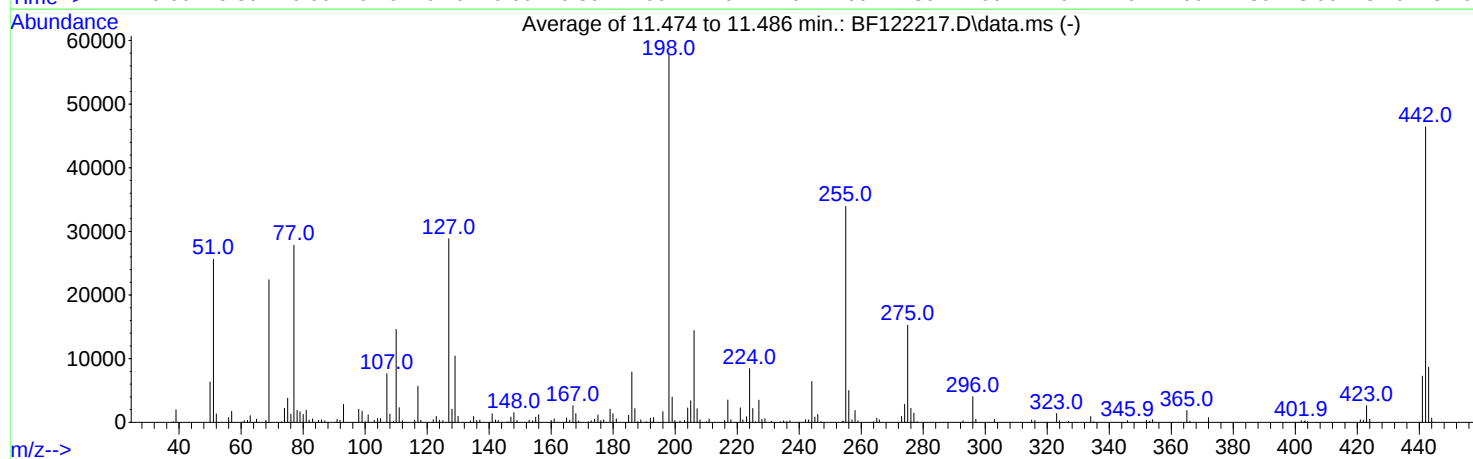


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF110220\  
 Data File : BF122217.D  
 Acq On : 2 Nov 2020 9:20  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF101220.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Oct 30 10:16:54 2020

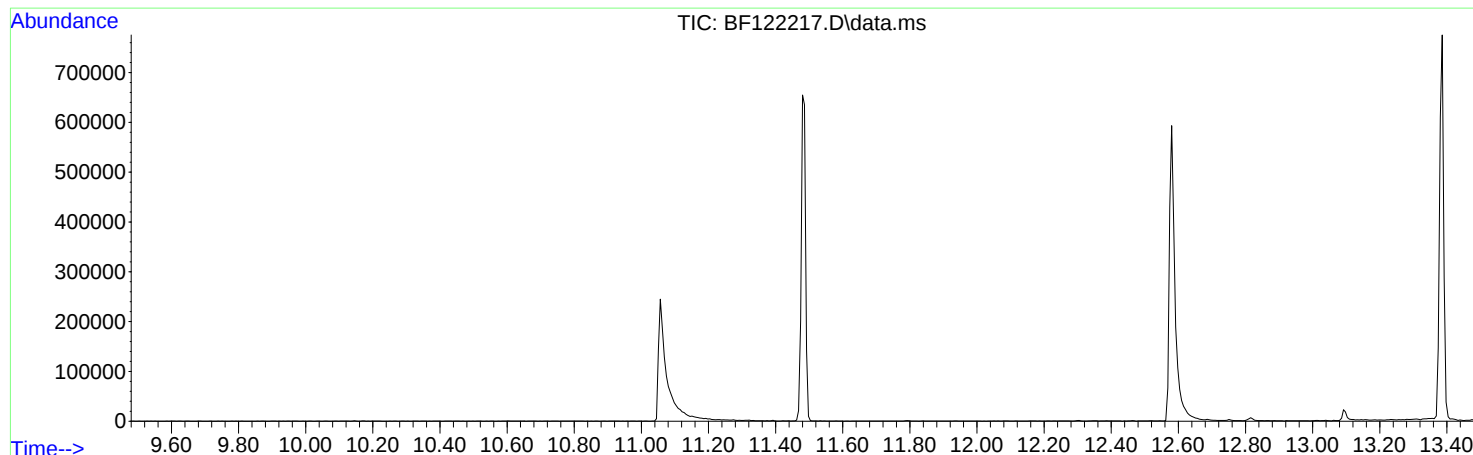

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 44.3         | 25631      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 322        | PASS                |
| 69             | 198             | 0.00            | 100             | 38.8         | 22399      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 49.9         | 28852      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 57797      | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 3981       | PASS                |
| 275            | 198             | 10              | 60              | 26.4         | 15287      | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 1871       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.6         | 7257       | PASS                |
| 442            | 198             | 50              | 100             | 80.4         | 46443      | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 8675       | PASS                |