
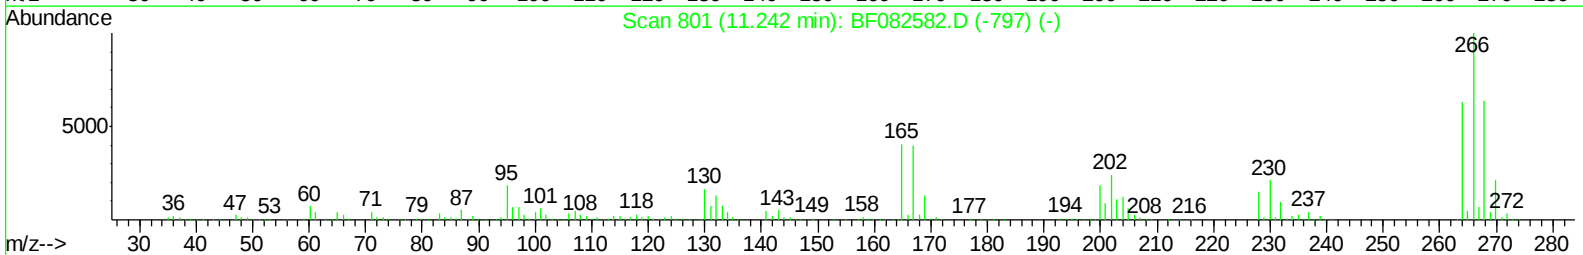
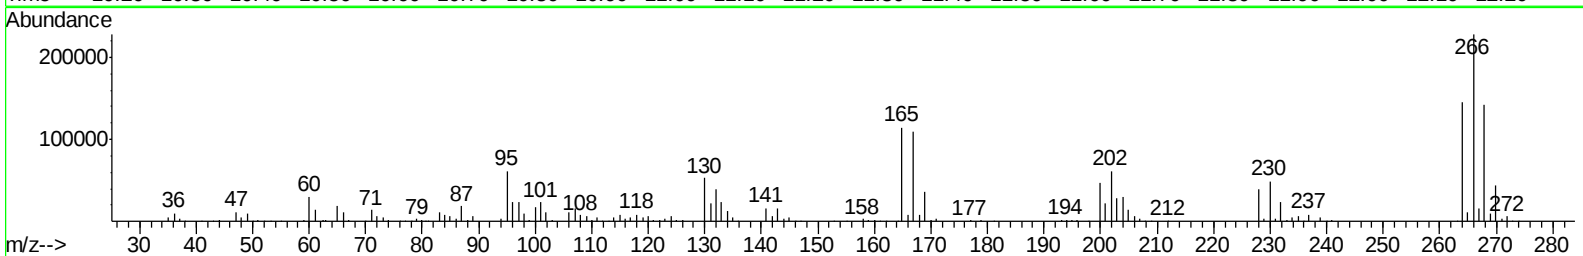


Data Path : Z:\HPCHEM1\BNA_F\Data\BF110315\
Data File : BF082654.D
Acq On : 3 Nov 2015 10:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 10:48:53 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

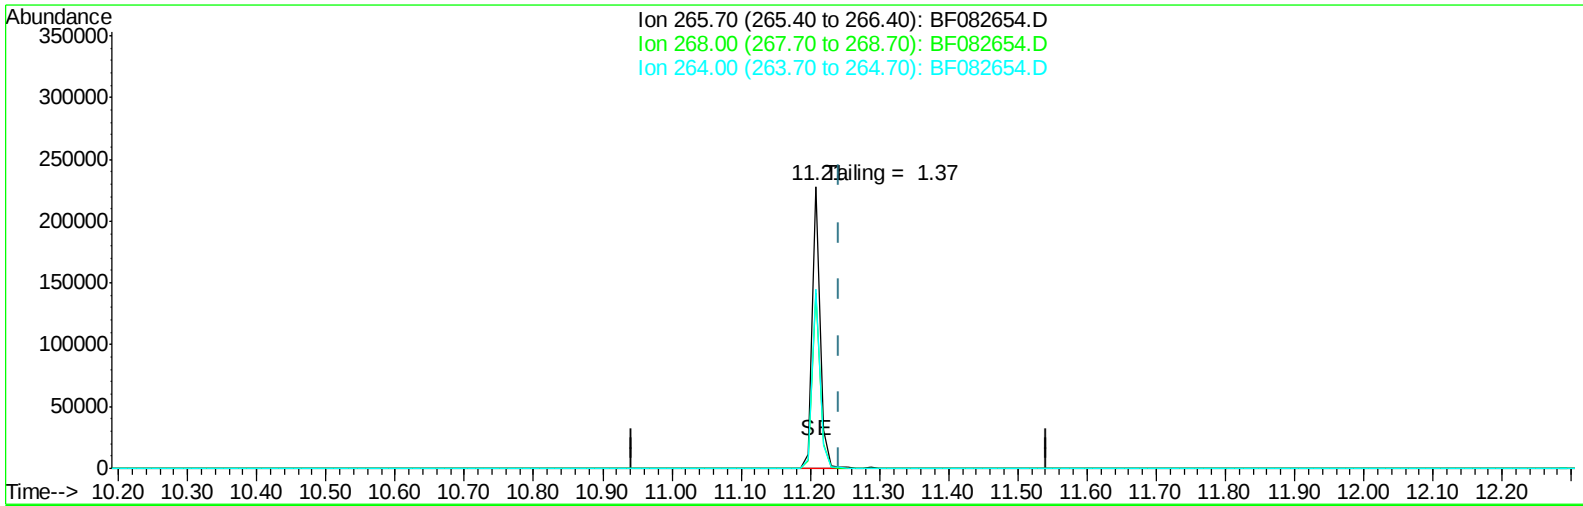

TIC: BF082654.D

(69) Pentachlorophenol (C)




11.208min (-0.034) 23038.89ng

response 181348

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.15
264.00	63.20	63.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF110315\
Data File : BF082654.D
Acq On : 3 Nov 2015 10:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 10:48:53 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

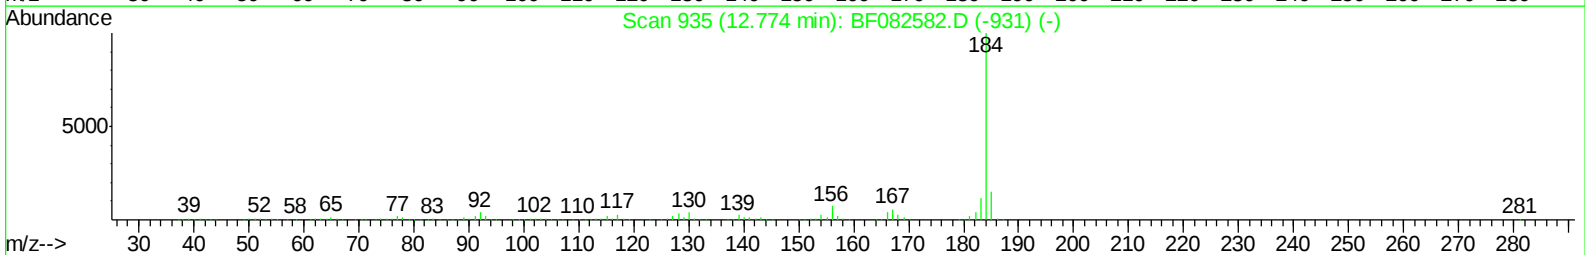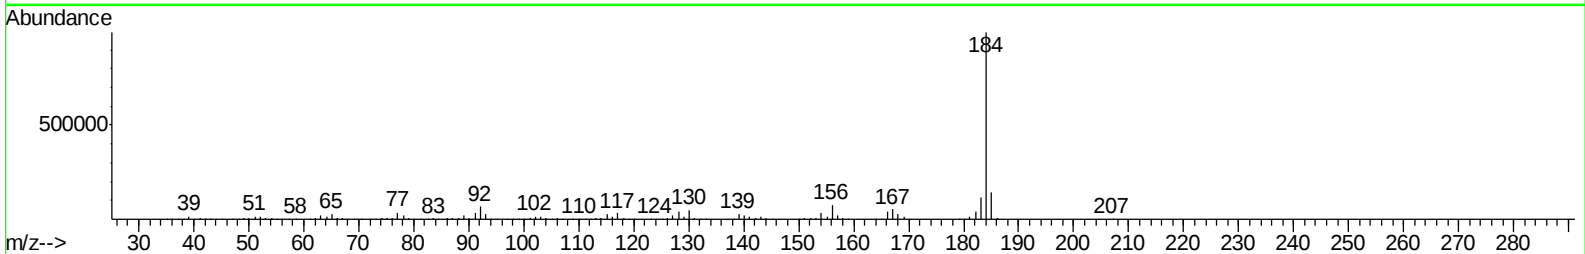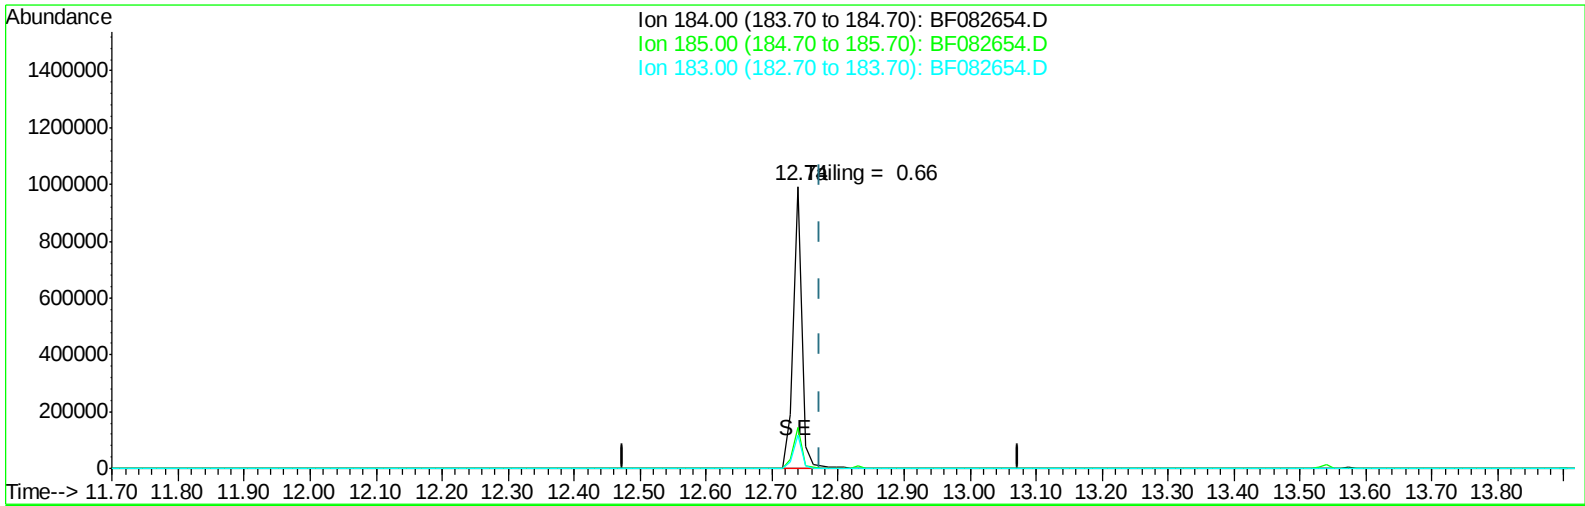

TIC: BF082654.D

(76) Benzidine

12.739min (-0.034) 0.00ng

response 893950

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.40
183.00	12.00	11.90
0.00	0.00	0.00