


Data Path : Z:\HPCHEM1\BNA F\Data\BF110315\
 Data File : BF082654.D
 Acq On : 3 Nov 2015 10:25
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 03 12:27:47 2015

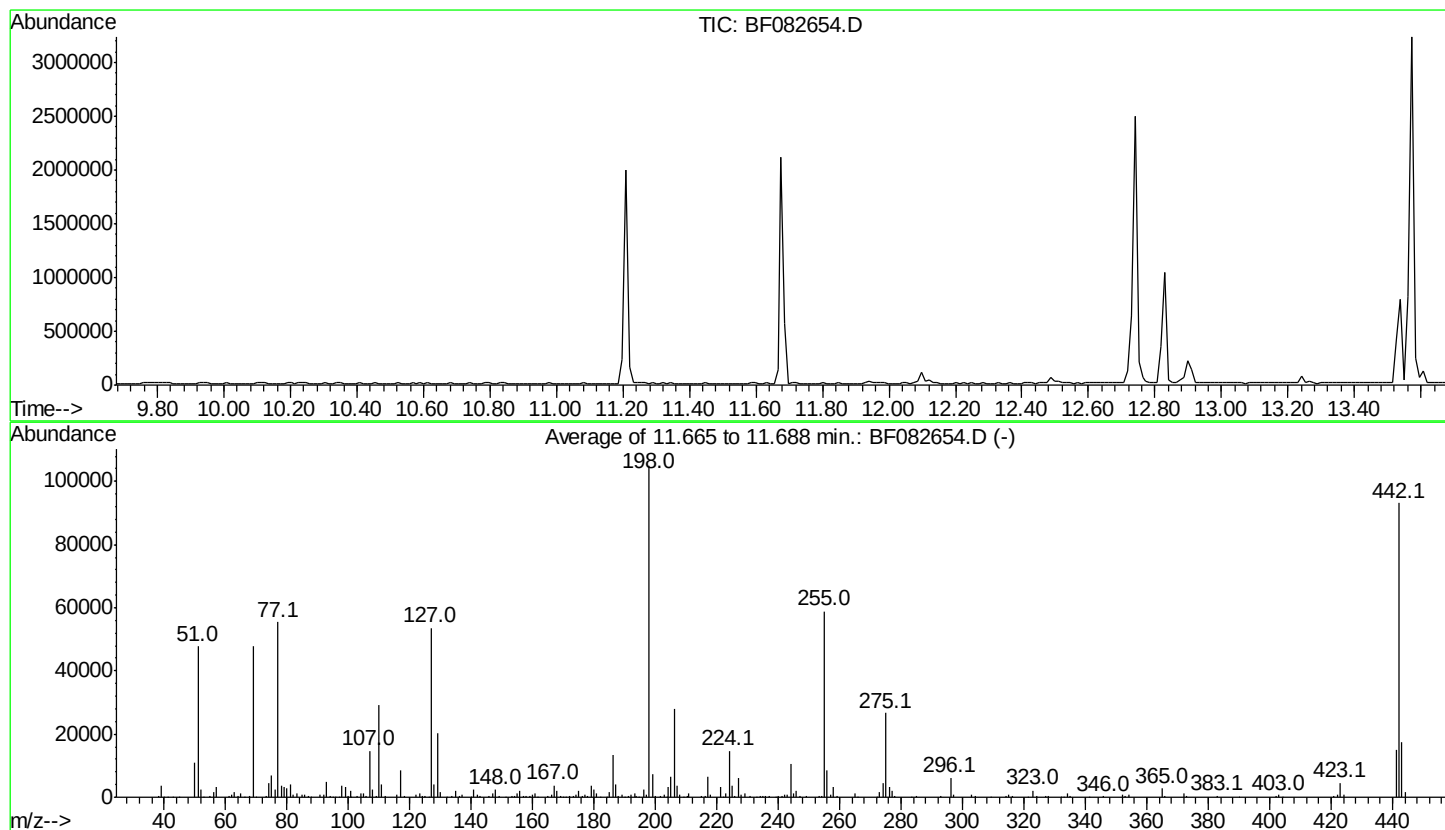

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	47747	PASS
68	69	0.00	2	1.1	534	PASS
69	198	0.00	100	45.7	47957	PASS
70	69	0.00	2	0.4	202	PASS
127	198	10	80	51.1	53656	PASS
197	198	0.00	2	0.7	769	PASS
198	198	100	100	100.0	105010	PASS
199	198	5	9	6.8	7184	PASS
275	198	10	60	25.3	26589	PASS
365	198	1	100	2.6	2753	PASS
441	442	0.01	24	16.2	15129	PASS
442	198	50	100	88.7	93194	PASS
443	442	15	24	18.6	17290	PASS